


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040524\
Data File : BG060787.D
Acq On : 5 Apr 2024 8:52
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

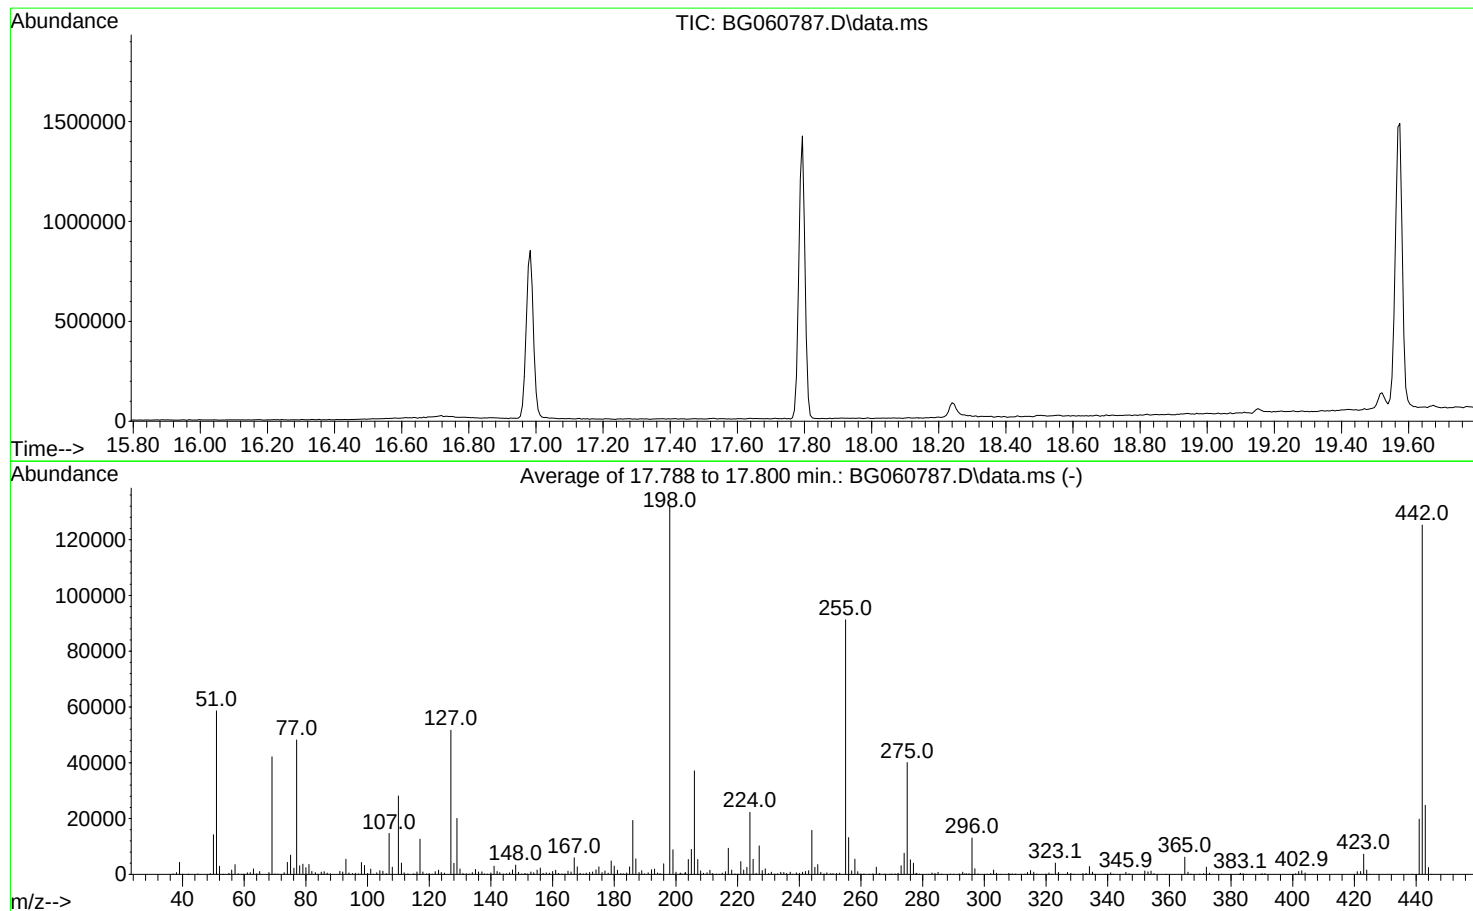




AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	44.4	58600	PASS
68	69	0.00	2	1.7	698	PASS
69	198	0.00	100	32.0	42181	PASS
70	69	0.00	2	0.5	203	PASS
127	198	10	80	39.2	51685	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	131869	PASS
199	198	5	9	6.7	8808	PASS
275	198	10	60	30.4	40101	PASS
365	198	1	100	4.7	6227	PASS
441	198	0.01	100	15.0	19789	PASS
442	442	50	100	100.0	125211	PASS
443	442	15	24	19.8	24800	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040524\
Data File : BG060787.D
Acq On : 5 Apr 2024 8:52
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 05 10:40:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

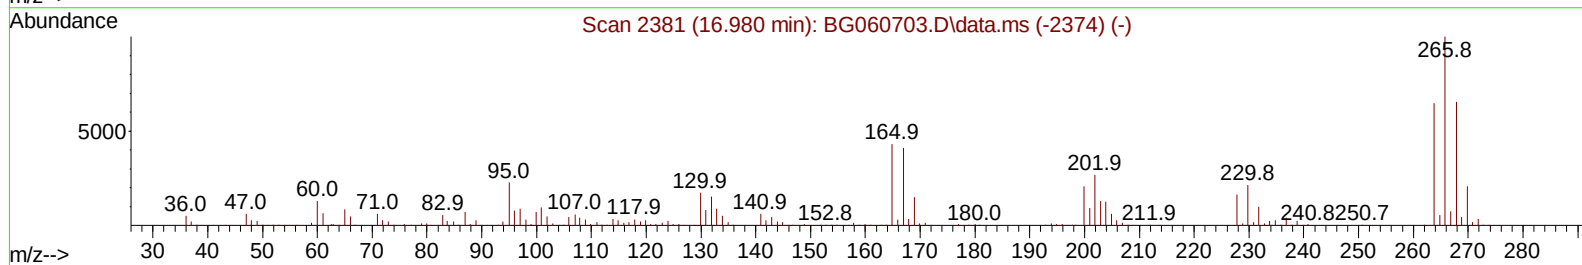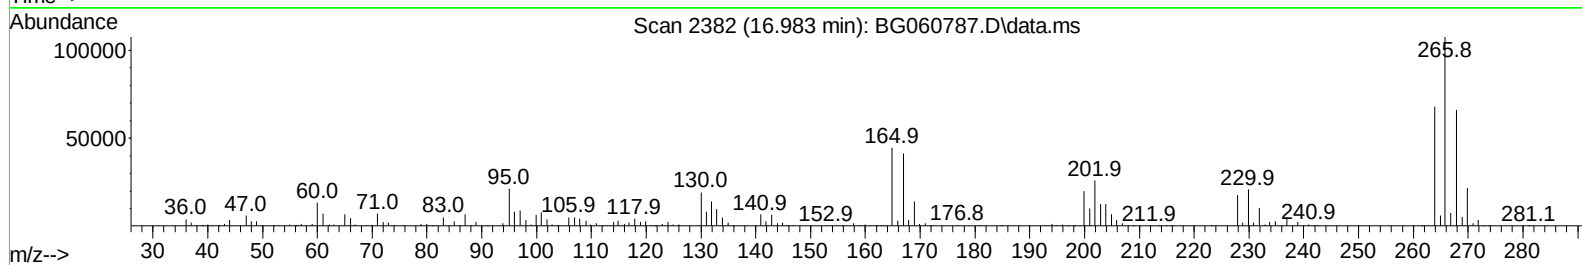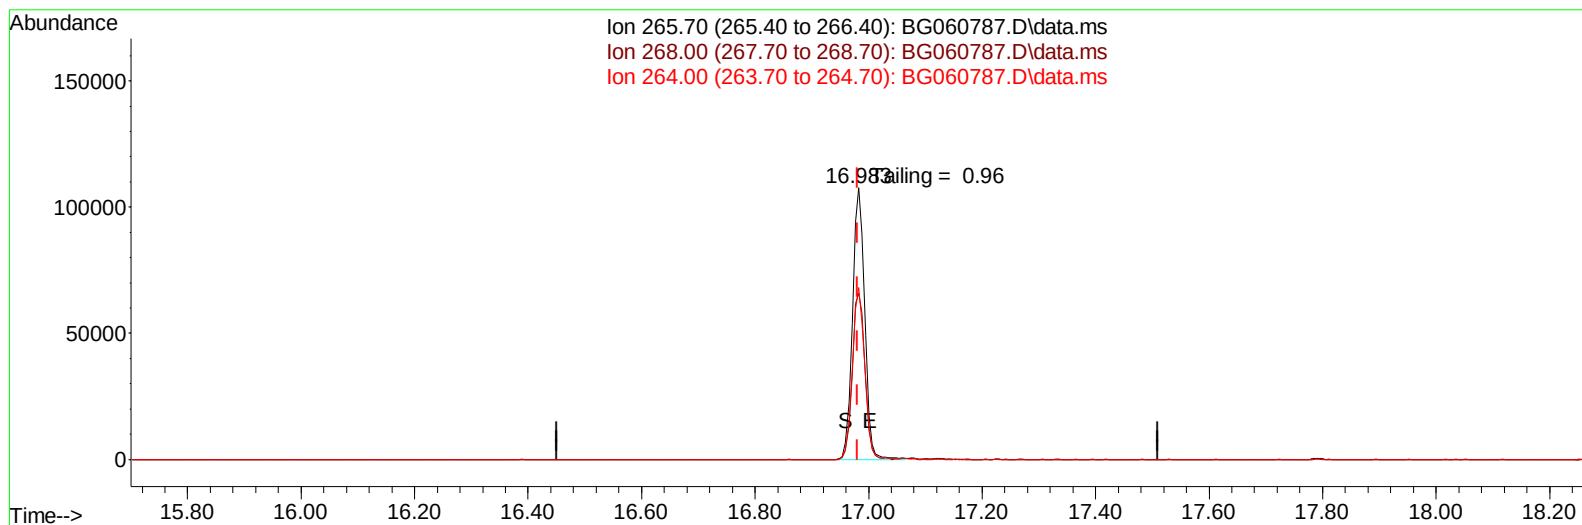

TIC: BG060787.D\data.ms

(70) Pentachlorophenol (C)

16.983min (+ 0.003) 317163.00 ng




response 161223

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	61.30
264.00	64.70	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040524\
Data File : BG060787.D
Acq On : 5 Apr 2024 8:52
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 05 10:40:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

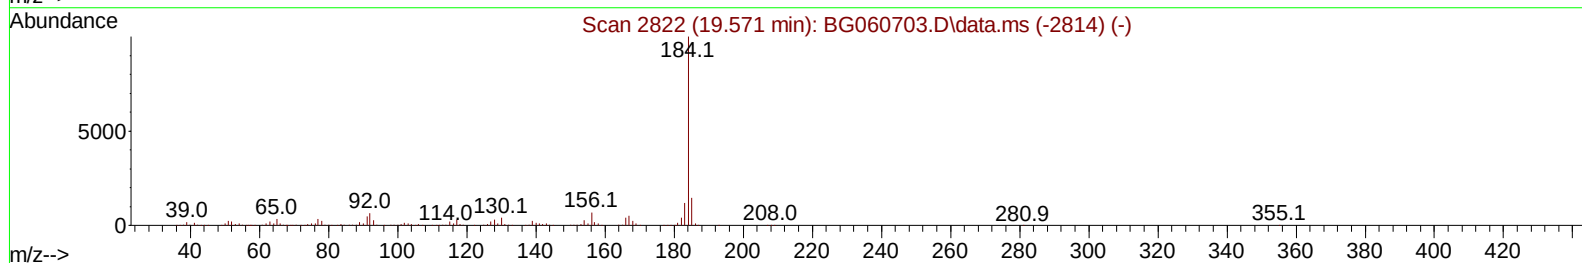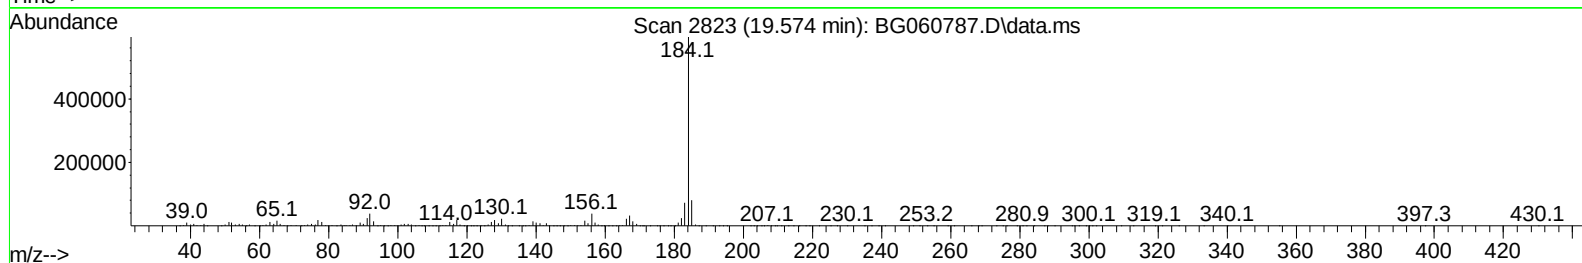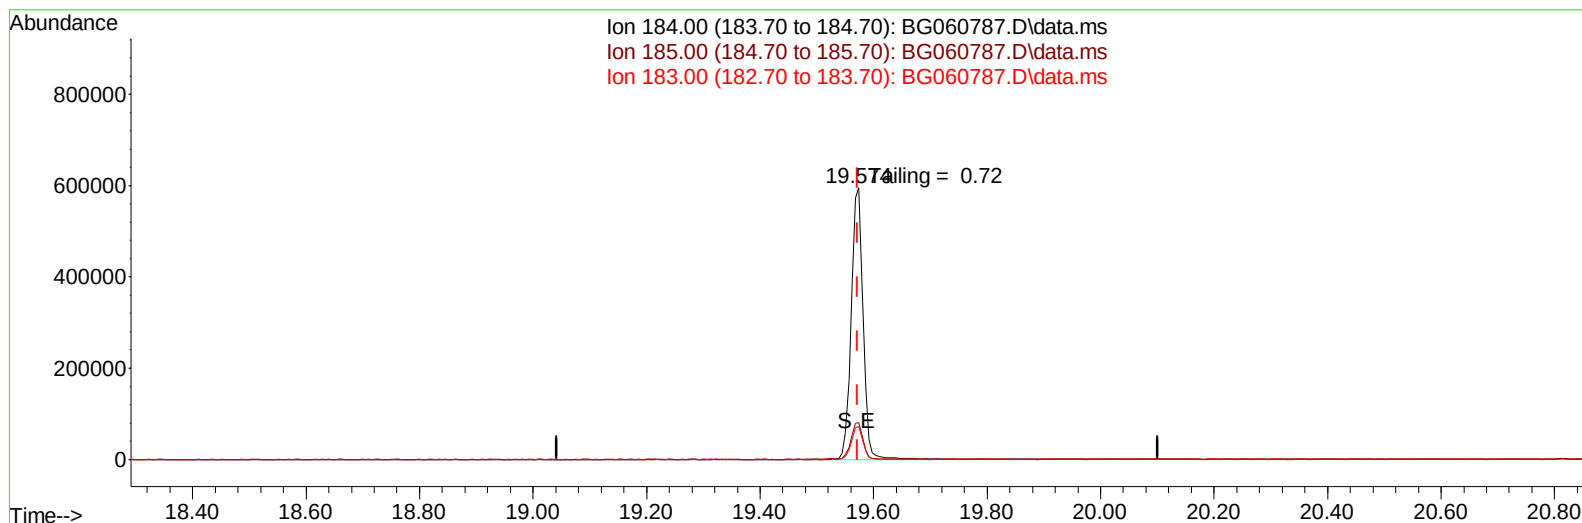

TIC: BG060787.D\data.ms

(77) Benzidine

19.574min (+ 0.003) 86077.11 ng

response 870373

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.49
183.00	11.90	12.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2024	BNA_G	<u>BG060787.D</u>
Compound Name	Response	Retention Time
DDT	485819	20.814
DDD	13890	20.373
DDE	922	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14812	500631	2.96

Instrument :
BNA_G
ClientSampleId :
DFTPP