


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG040720\
 Data File : BG044953.D
 Acq On : 7 Apr 2020 13:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Title : SVOA CALIBRATION
 Last Update : Tue Apr 07 11:04:24 2020

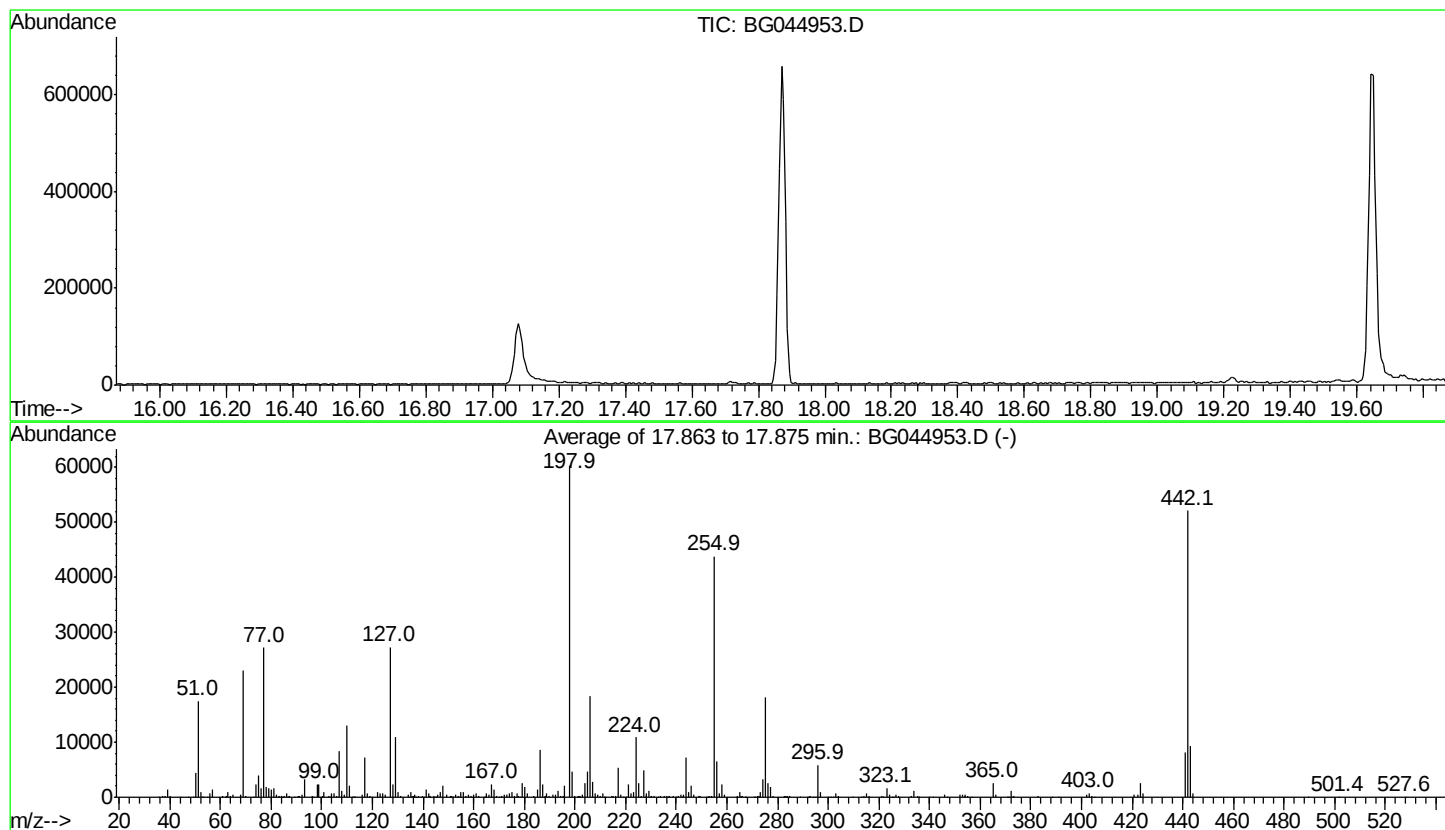

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	17479	PASS
68	69	0.00	2	1.6	381	PASS
69	198	0.00	100	38.4	23136	PASS
70	69	0.00	2	0.8	176	PASS
127	198	10	80	45.2	27269	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60269	PASS
199	198	5	9	7.7	4641	PASS
275	198	10	60	30.1	18146	PASS
365	198	1	100	4.3	2603	PASS
441	198	0.01	100	13.5	8162	PASS
442	198	50	100	86.5	52104	PASS
443	442	15	24	18.1	9419	PASS