
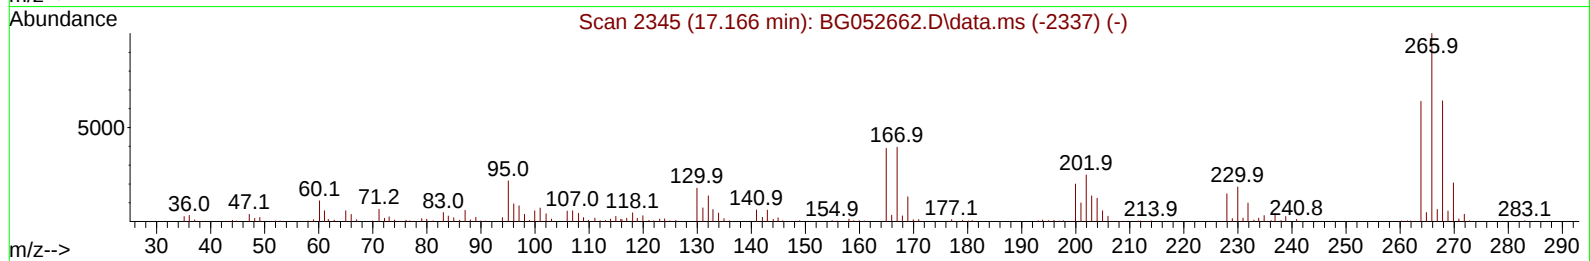
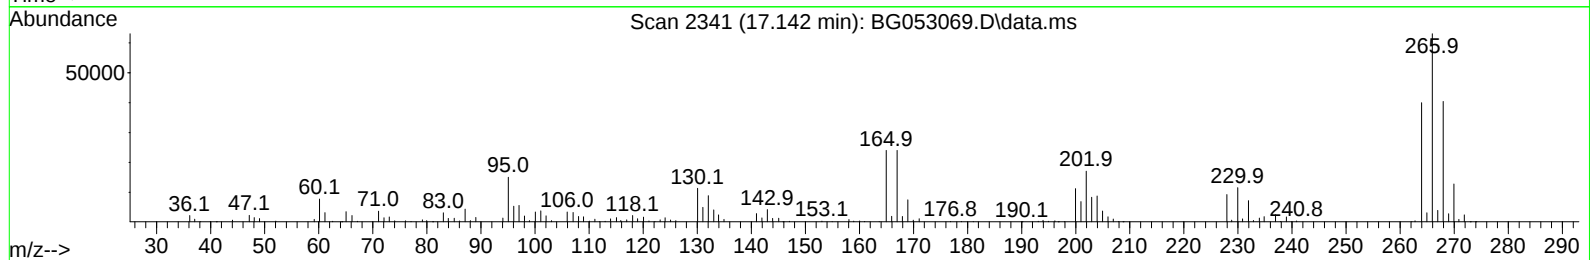


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040722\
 Data File : BG053069.D
 Acq On : 7 Apr 2022 10:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 07:39:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 06 14:35:39 2022
 Response via : Initial Calibration

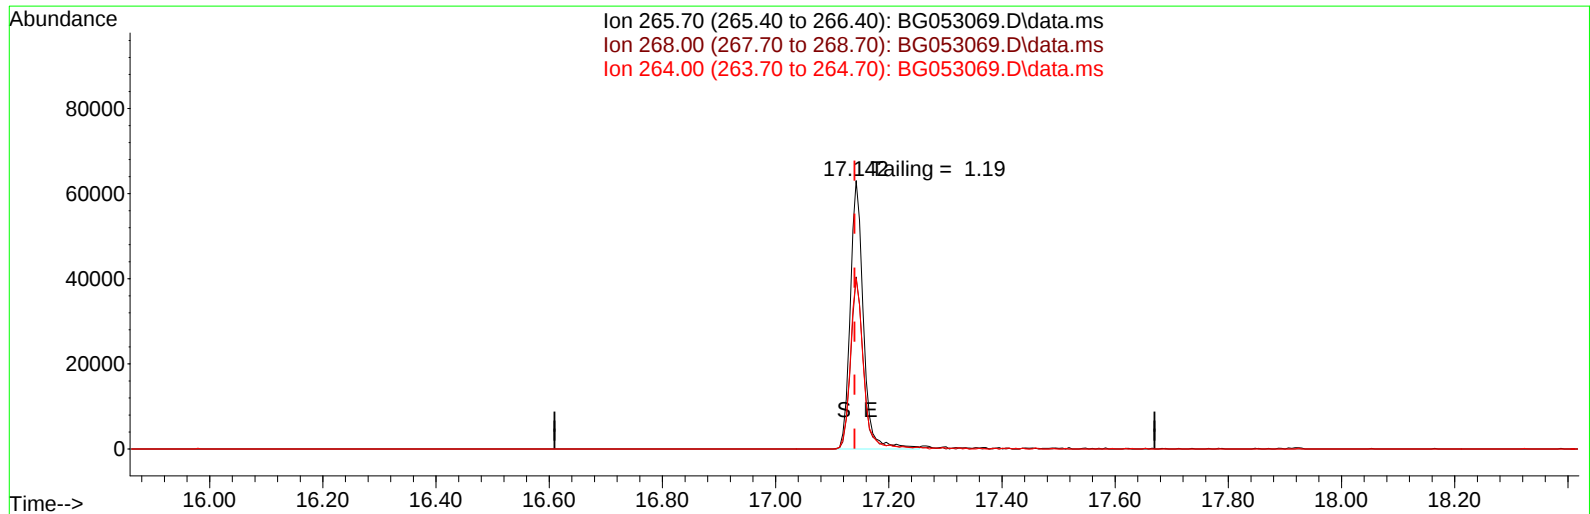

TIC: BG053069.D\data.ms

(70) Pentachlorophenol (C)




17.142min (+ 0.003) 96962.92 ng

response 99781

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	64.09
264.00	56.60	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040722\
 Data File : BG053069.D
 Acq On : 7 Apr 2022 10:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 07:39:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 06 14:35:39 2022
 Response via : Initial Calibration

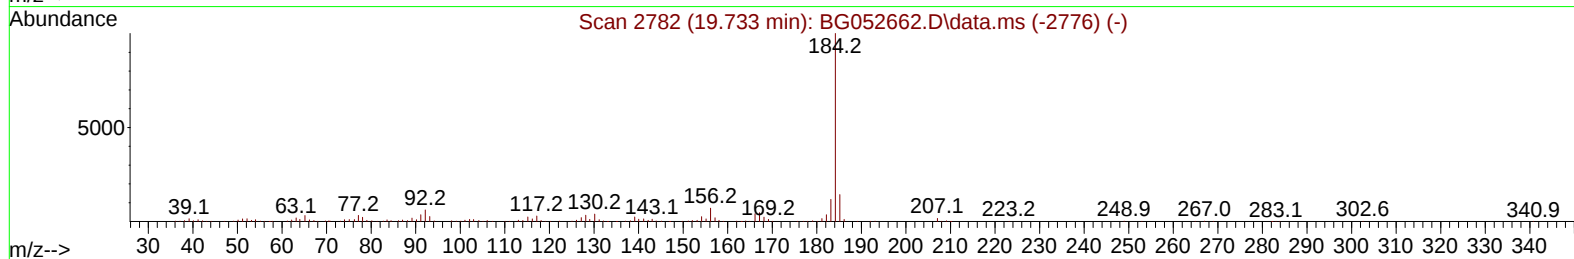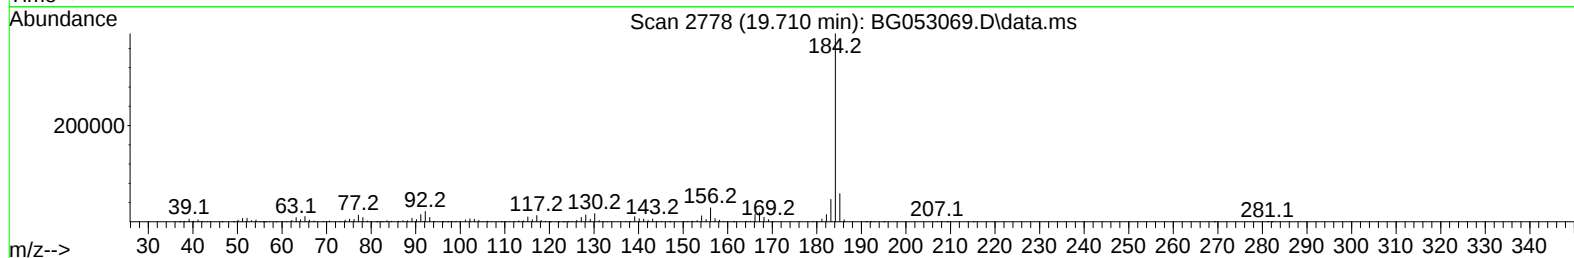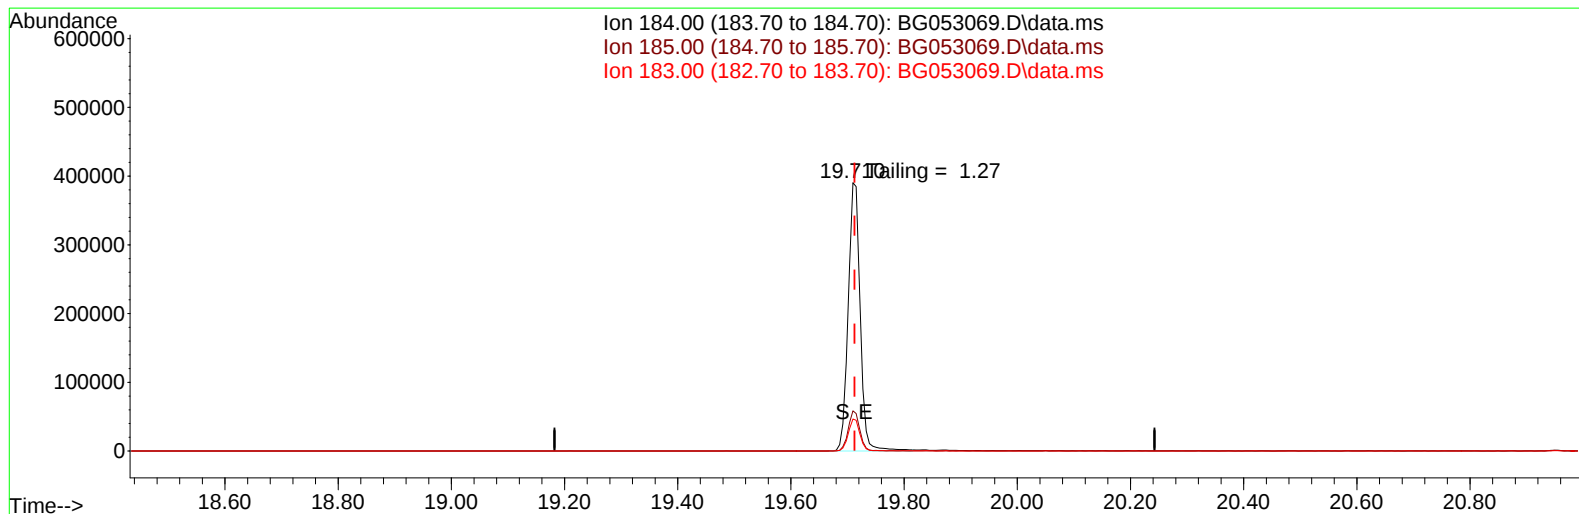

TIC: BG053069.D\data.ms

(77) Benzidine**19.710min (-0.003) 413715.64 ng****response 576210**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.98
183.00	11.80	11.94
0.00	0.00	0.00