

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040722\
 Data File : BG053071.D
 Acq On : 7 Apr 2022 13:05
 Operator : CG/JU
 Sample : PB143883BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB143883BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.693	385	392	401	rBV	600264	994370	31.90%	8.347%
2	7.285	655	663	676	rBV	655048	1136329	36.46%	9.538%
3	8.125	799	806	814	rBV2	111275	198100	6.36%	1.663%
4	9.288	994	1004	1013	rBV	396695	727283	23.33%	6.105%
5	10.939	1275	1285	1295	rBV	156602	276178	8.86%	2.318%
6	13.371	1692	1699	1707	rBV	1086821	1723827	55.30%	14.470%
7	14.746	1926	1933	1941	rBV	263722	427802	13.72%	3.591%
8	16.232	2179	2186	2202	rBV	986546	1534601	49.23%	12.881%
9	17.489	2393	2400	2409	rBV	372015	575693	18.47%	4.832%
10	20.097	2837	2844	2851	rBV	2309305	3117029	100.00%	26.164%
11	21.777	3123	3130	3138	rBV	346374	595276	19.10%	4.997%
12	25.085	3682	3693	3708	rVB2	205017	606769	19.47%	5.093%




Sum of corrected areas: 11913257

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040722\
Data File : BG053071.D
Acq On : 7 Apr 2022 13:05
Operator : CG/JU
Sample : PB143883BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143883BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

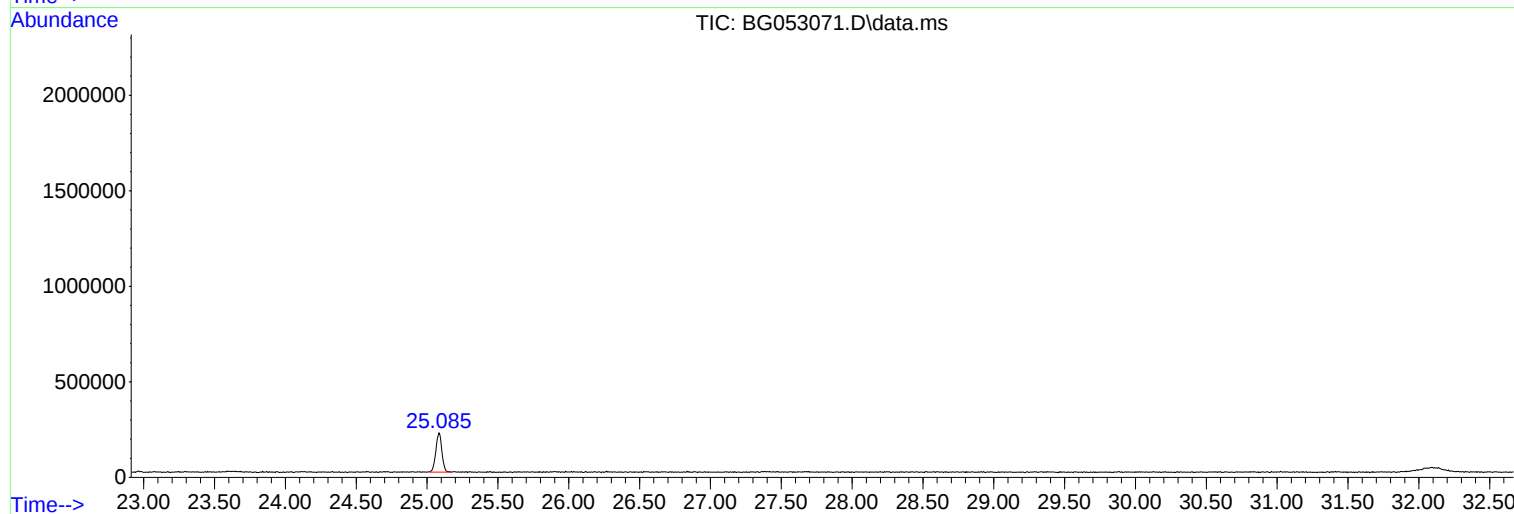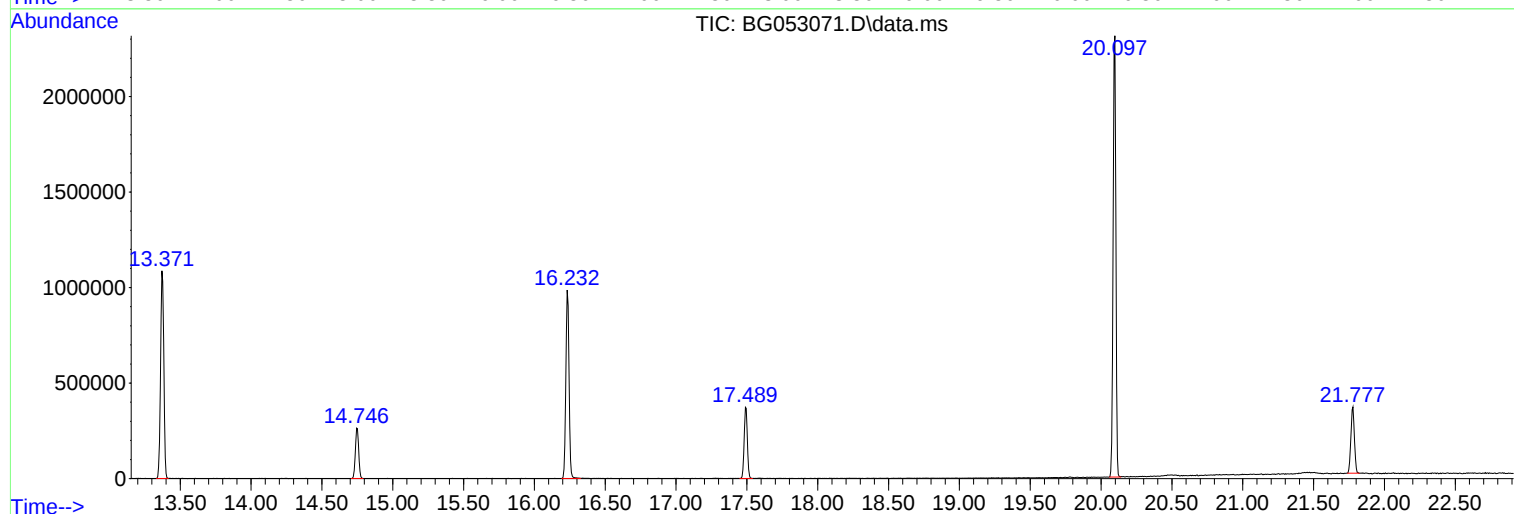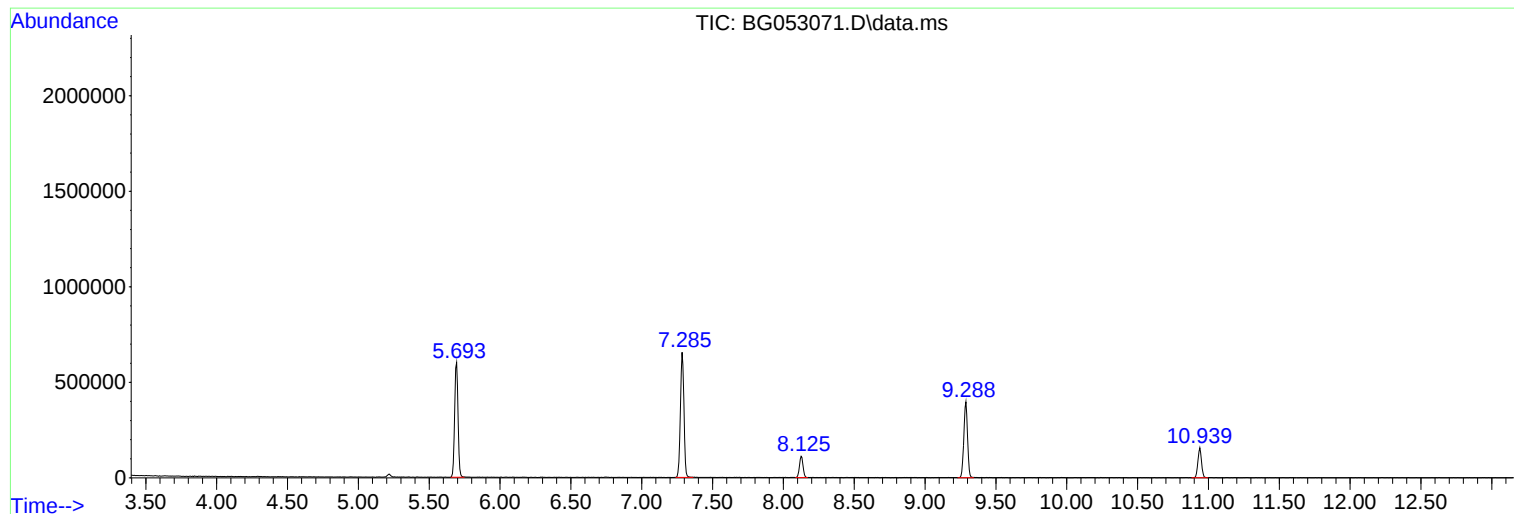

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040722\
Data File : BG053071.D
Acq On : 7 Apr 2022 13:05
Operator : CG/JU
Sample : PB143883BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143883BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040722\
Data File : BG053071.D
Acq On : 7 Apr 2022 13:05
Operator : CG/JU
Sample : PB143883BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143883BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------