


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040722\
 Data File : BG053069.D
 Acq On : 7 Apr 2022 10:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 06 14:35:39 2022

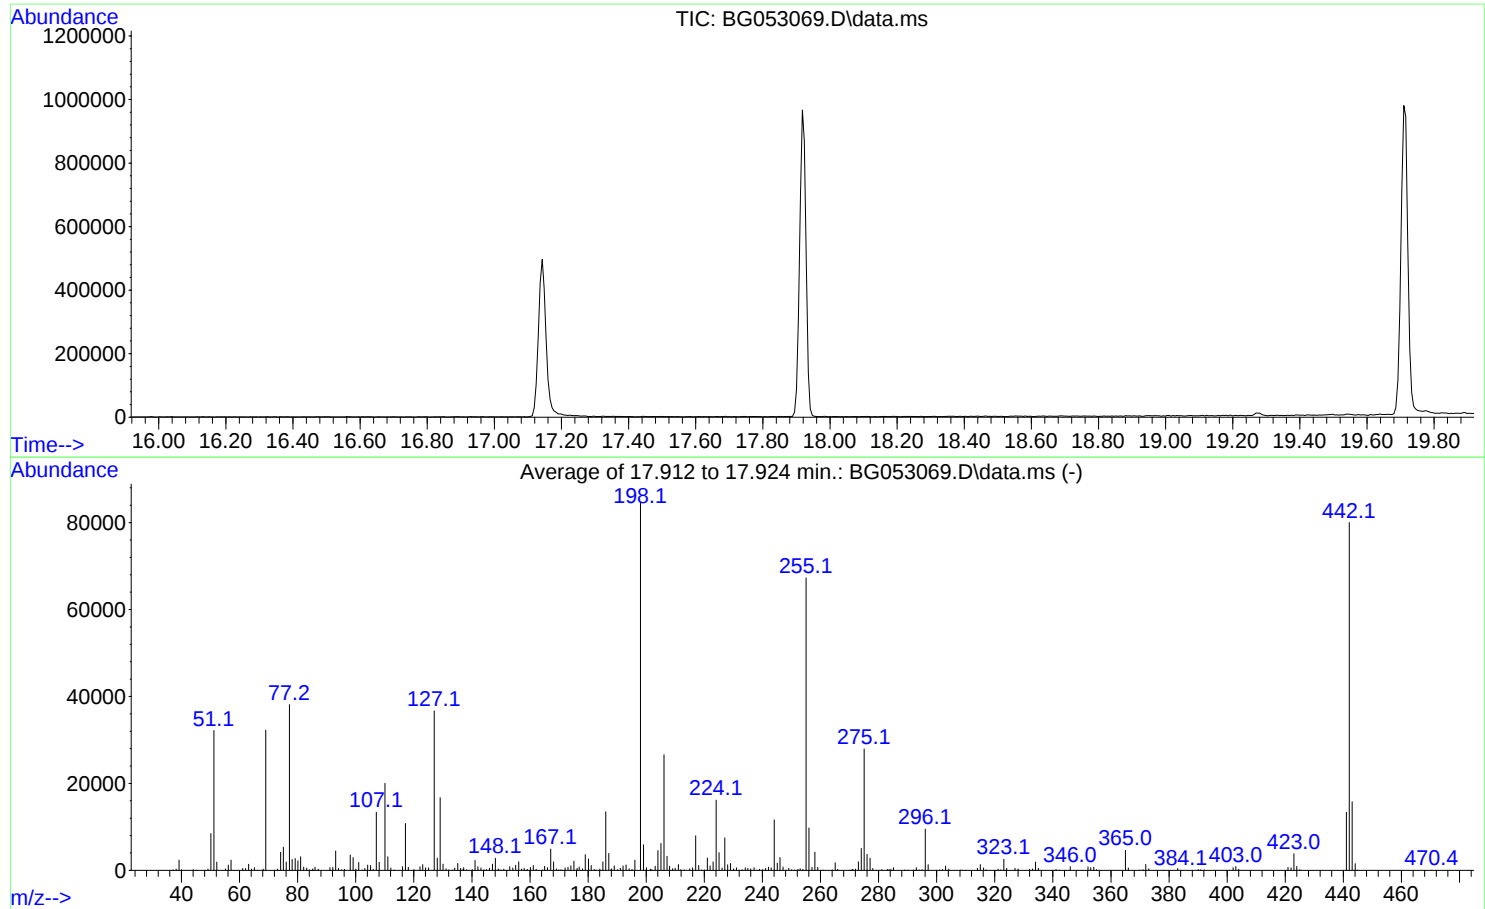


AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	32160	PASS
68	69	0.00	2	0.9	304	PASS
69	198	0.00	100	38.1	32245	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.4	36712	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84627	PASS
199	198	5	9	7.0	5897	PASS
275	198	10	60	33.0	27949	PASS
365	198	1	100	5.4	4611	PASS
441	198	0.01	100	15.8	13366	PASS
442	442	50	100	100.0	80037	PASS
443	442	15	24	19.7	15802	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040722\
 Data File : BG053069.D
 Acq On : 7 Apr 2022 10:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 08 07:39:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 06 14:35:39 2022
 Response via : Initial Calibration

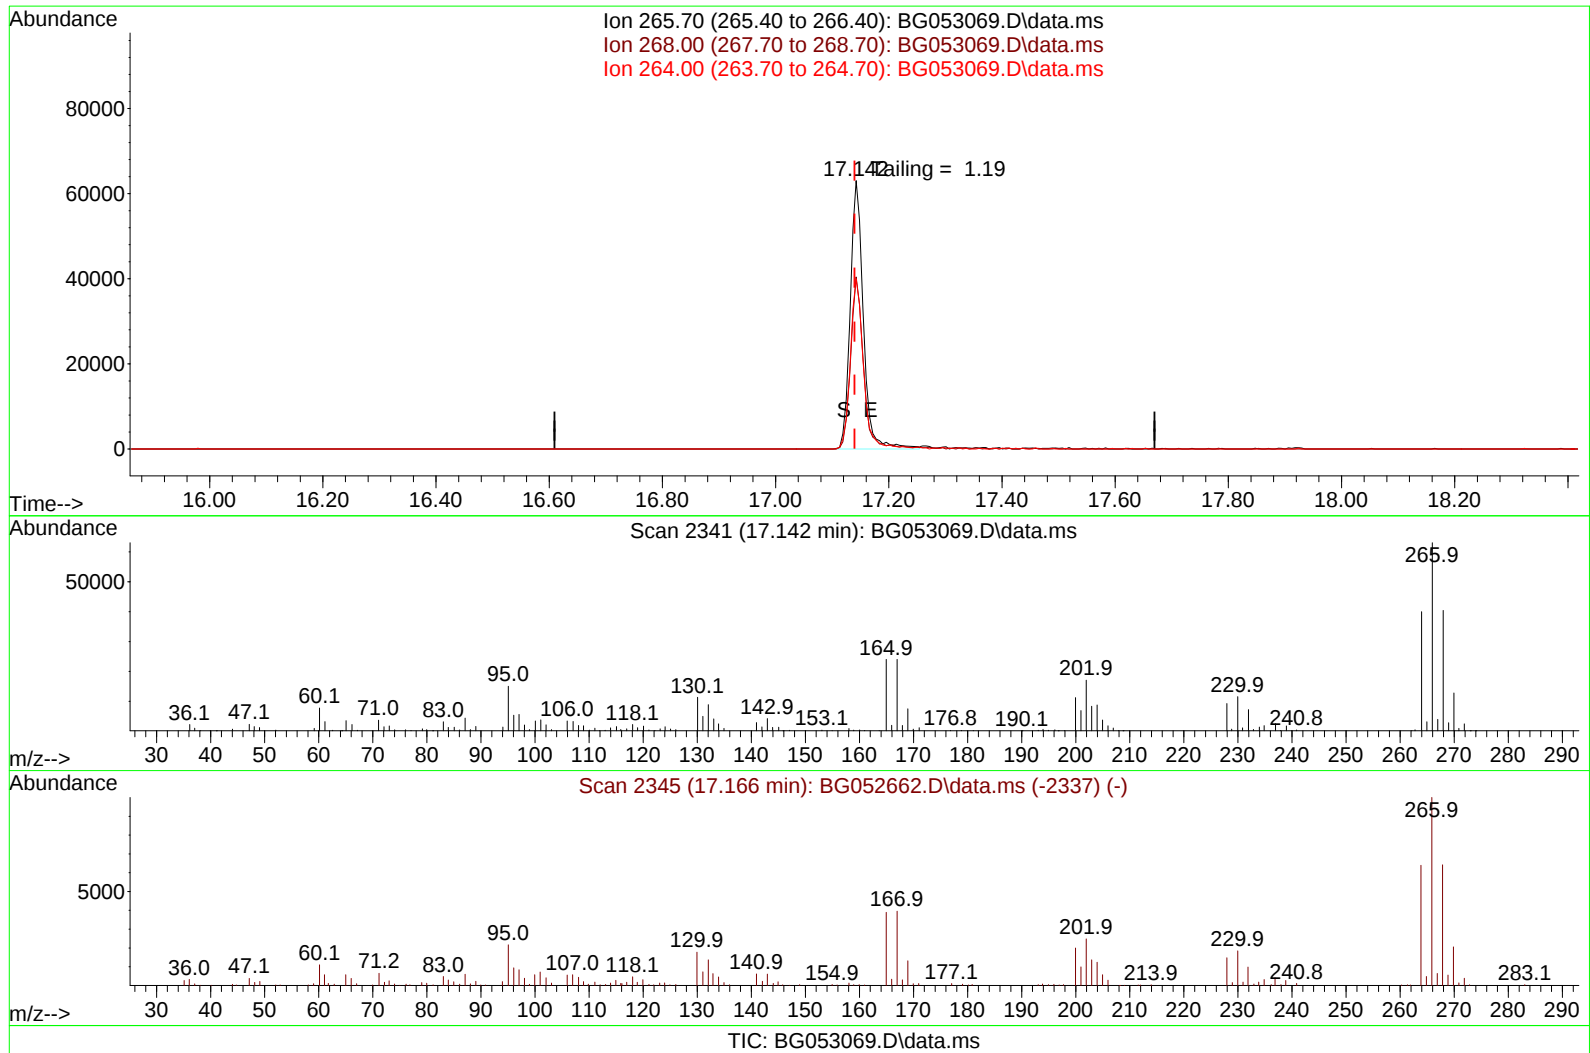

(70) Pentachlorophenol (C)

17.142min (+ 0.003) 96962.92 ng




response 99781

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	64.09
264.00	56.60	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040722\
Data File : BG053069.D
Acq On : 7 Apr 2022 10:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 08 07:39:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 14:35:39 2022
Response via : Initial Calibration

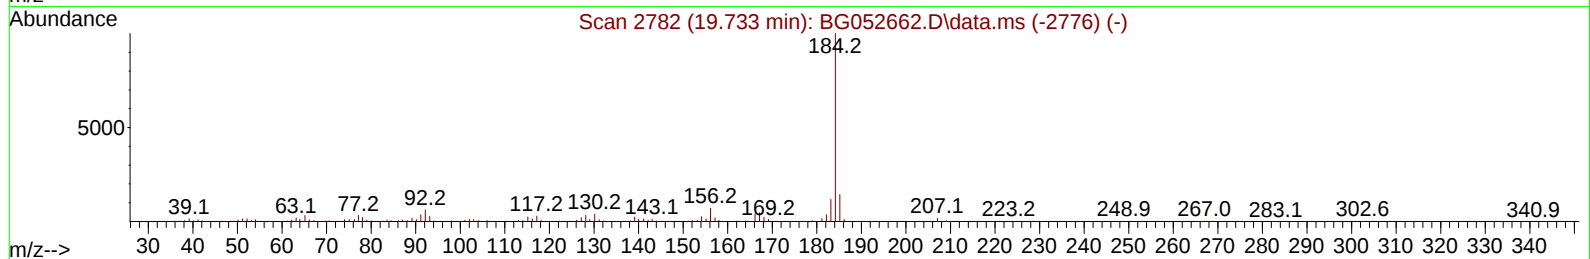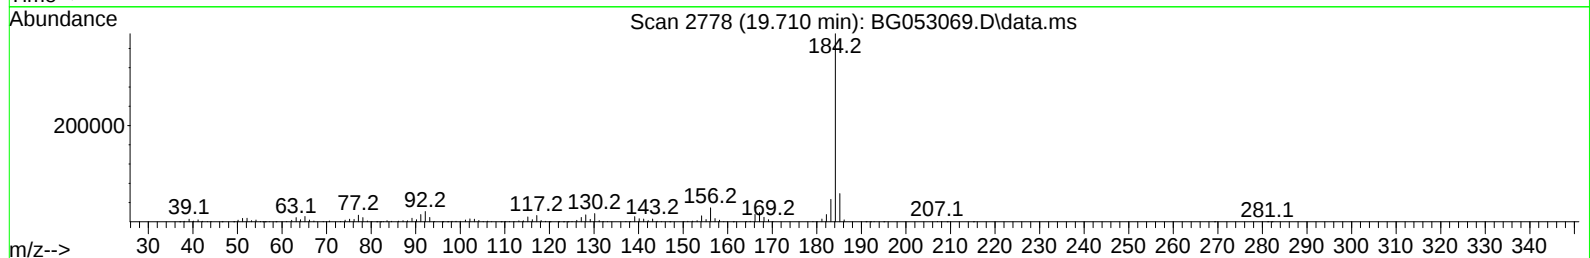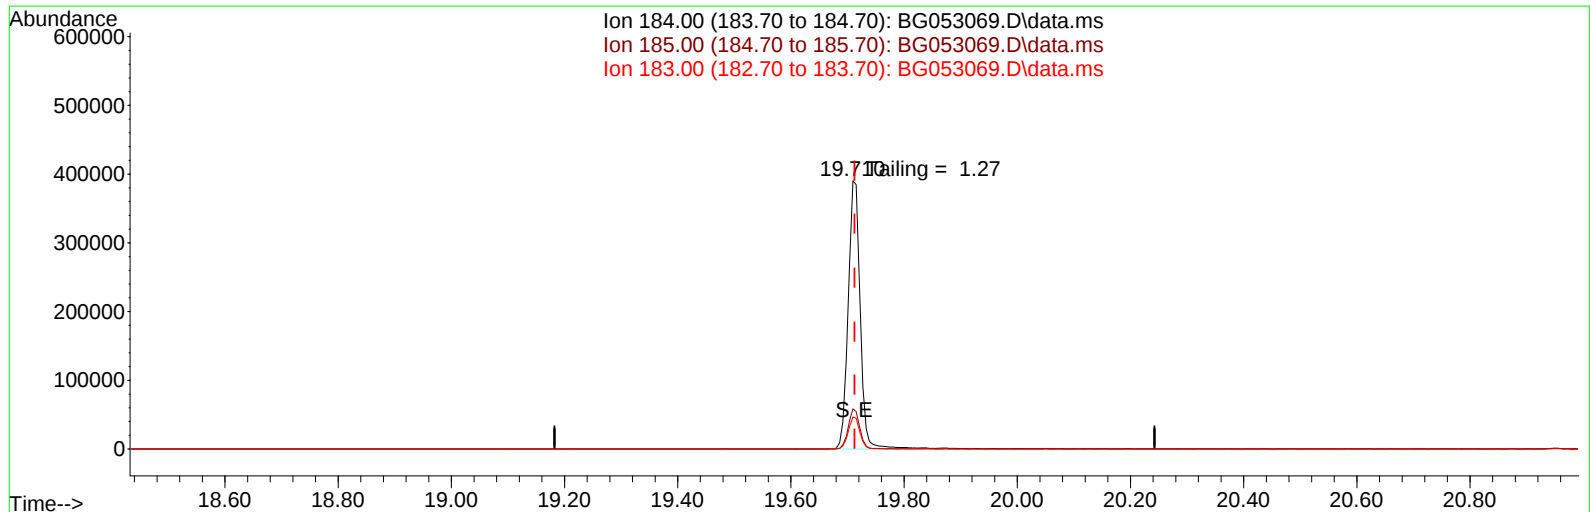

TIC: BG053069.D\data.ms

(77) Benzidine

19.710min (-0.003) 413715.64 ng

response 576210

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.98
183.00	11.80	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/7/2022	BNA_G	<u>BG053069.D</u>
Compound Name	Response	Retention Time
DDT	297031	20.949
DDD	9079	20.503
DDE	499	20.003
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9578	306609	3.12

Instrument :
BNA_G
ClientSampleId :
DFTPP