
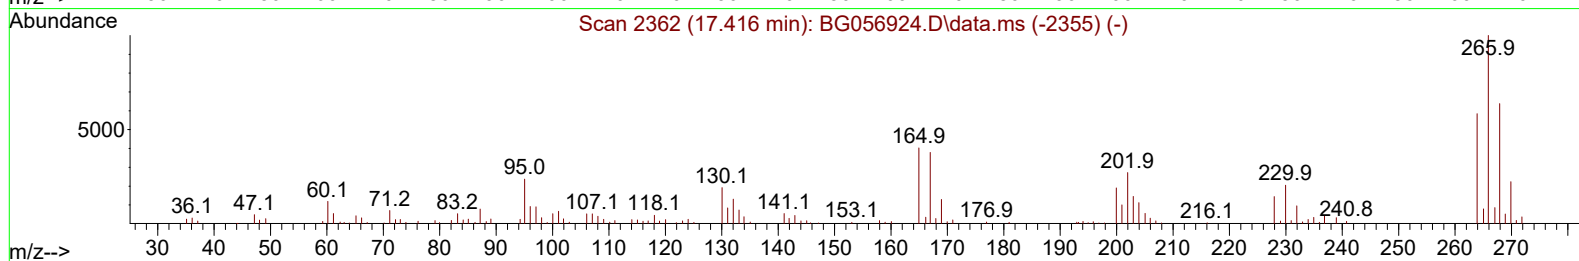
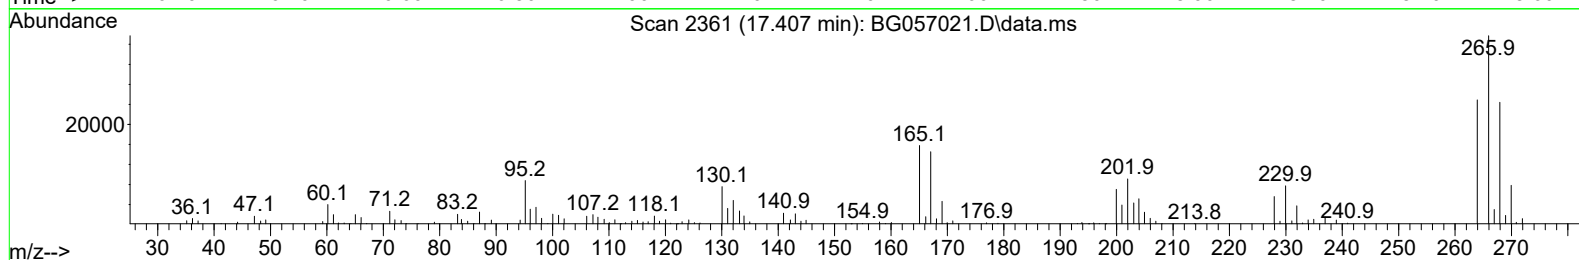


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057021.D
Acq On : 7 Apr 2023 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 05:05:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 04:45:47 2023
Response via : Initial Calibration

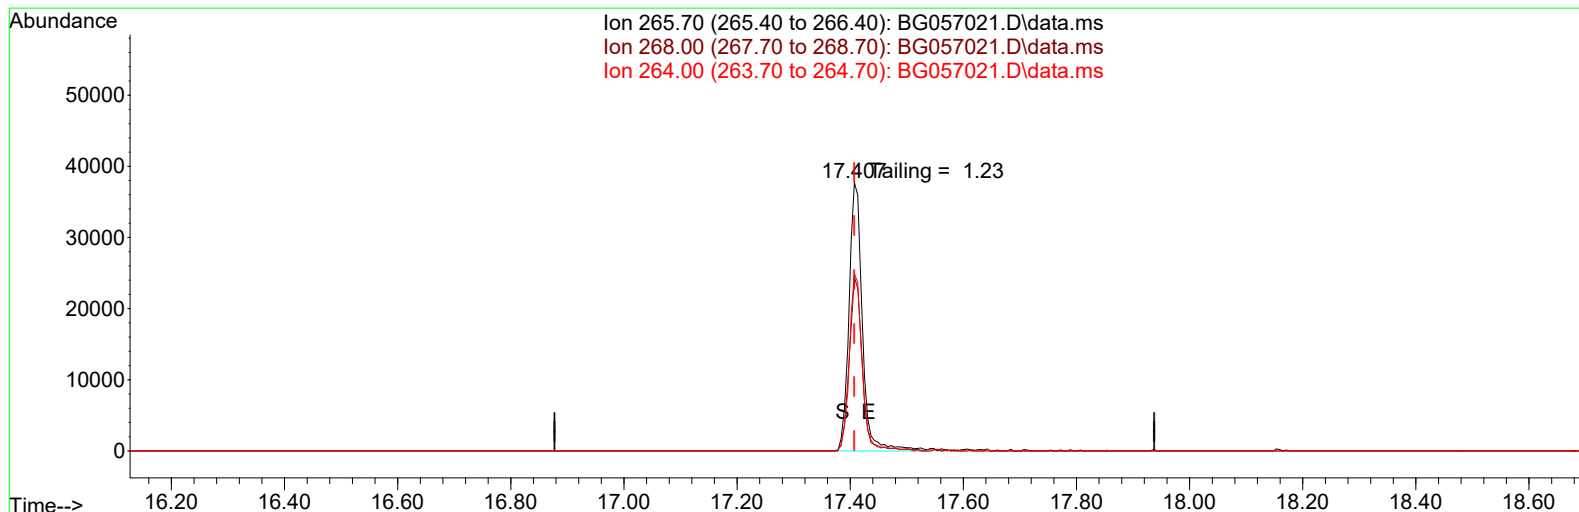

TIC: BG057021.D\data.ms

(70) Pentachlorophenol (C)




17.407min (+ 0.000) 29440.12 ng

response 62008

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.78
264.00	58.50	65.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057021.D
Acq On : 7 Apr 2023 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 05:05:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 04:45:47 2023
Response via : Initial Calibration

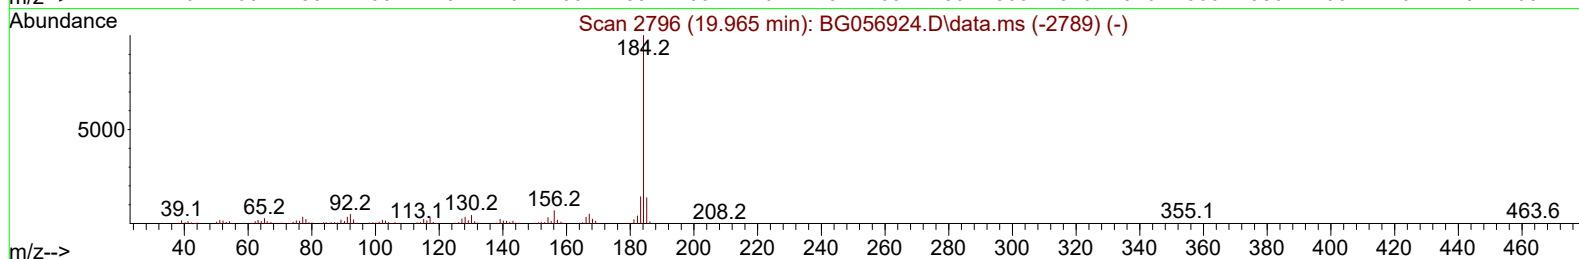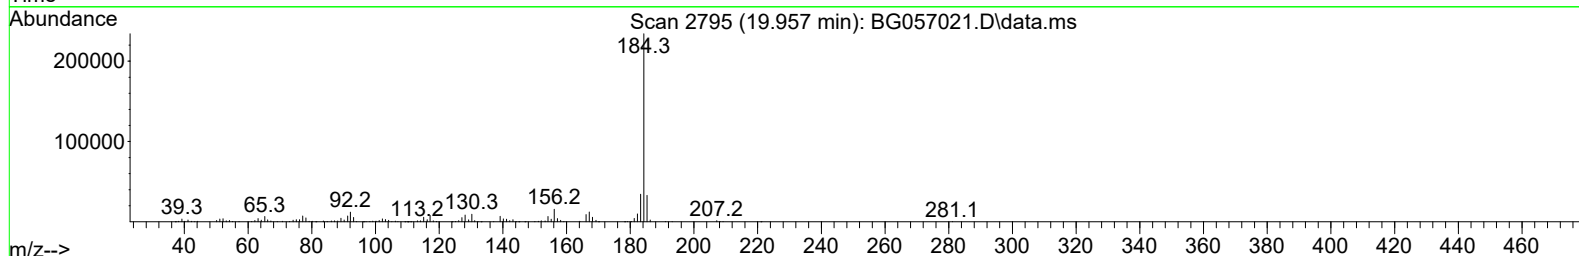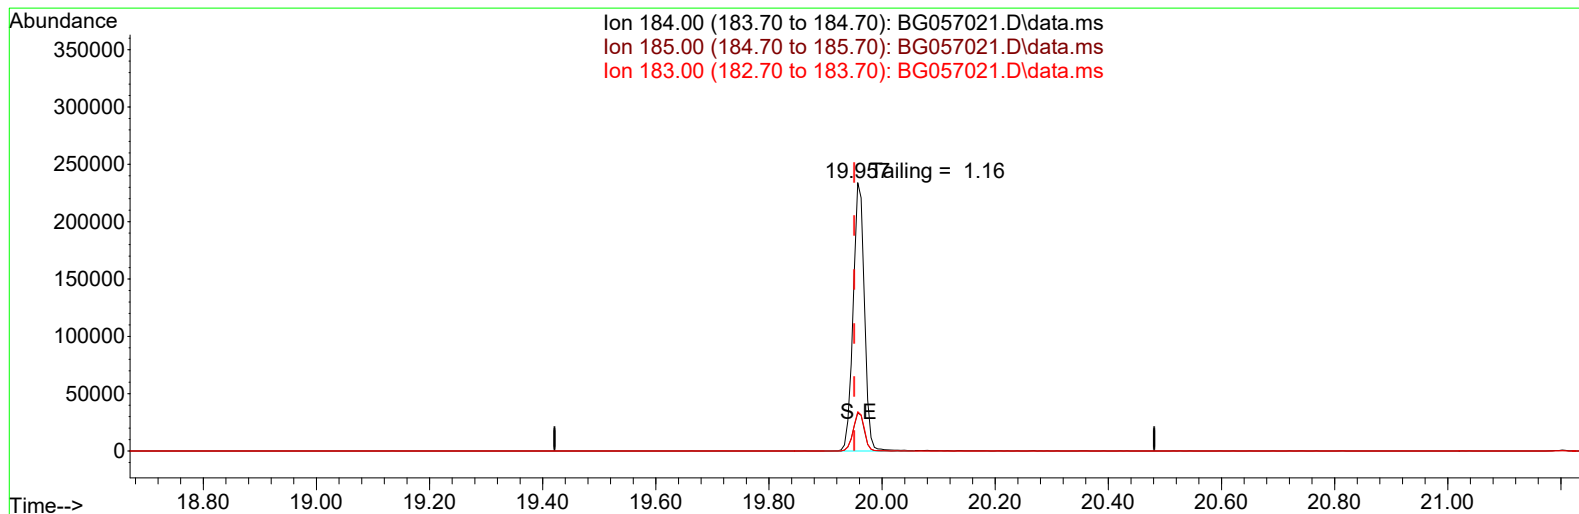

TIC: BG057021.D\data.ms

(77) Benzidine

19.957min (+ 0.006) 0.00 ng m

response 324614

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.13
183.00	14.20	14.70
0.00	0.00	0.00