

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
 Data File : BG057028.D
 Acq On : 7 Apr 2023 15:58
 Operator : CG/JU
 Sample : 02224-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU3-FC-BACKFILL-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057028.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.438	317	323	331	rBB	82255	131928	13.56%	3.086%
2	5.914	398	404	413	rBB	196397	323180	33.22%	7.560%
3	7.535	673	680	688	rBV	212392	369400	37.98%	8.642%
4	8.405	822	828	835	rBB	47353	75934	7.81%	1.776%
5	9.585	1021	1029	1037	rVB	121100	223106	22.94%	5.219%
6	11.248	1305	1312	1320	rVB	60551	108340	11.14%	2.534%
7	13.645	1713	1720	1727	rVB	383055	582032	59.83%	13.616%
8	15.019	1948	1954	1961	rBV	114473	171167	17.60%	4.004%
9	16.353	2175	2181	2188	rBV2	14701	20914	2.15%	0.489%
10	16.500	2199	2206	2214	rVB	320266	480229	49.37%	11.234%
11	17.757	2414	2420	2426	rBV	148664	223190	22.94%	5.221%
12	18.591	2557	2562	2570	rBV3	21238	30151	3.10%	0.705%
13	19.848	2771	2776	2783	rBV7	6016	10602	1.09%	0.248%
14	20.324	2852	2857	2863	rBV	728907	972742	100.00%	22.756%
15	21.640	3076	3081	3089	rVB3	34240	59407	6.11%	1.390%
16	22.074	3149	3155	3165	rBV2	133823	234611	24.12%	5.488%
17	22.891	3288	3294	3299	rBV9	5542	13961	1.44%	0.327%
18	25.617	3745	3758	3768	rVB2	77762	243788	25.06%	5.703%




Sum of corrected areas: 4274682

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057028.D
Acq On : 7 Apr 2023 15:58
Operator : CG/JU
Sample : 02224-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

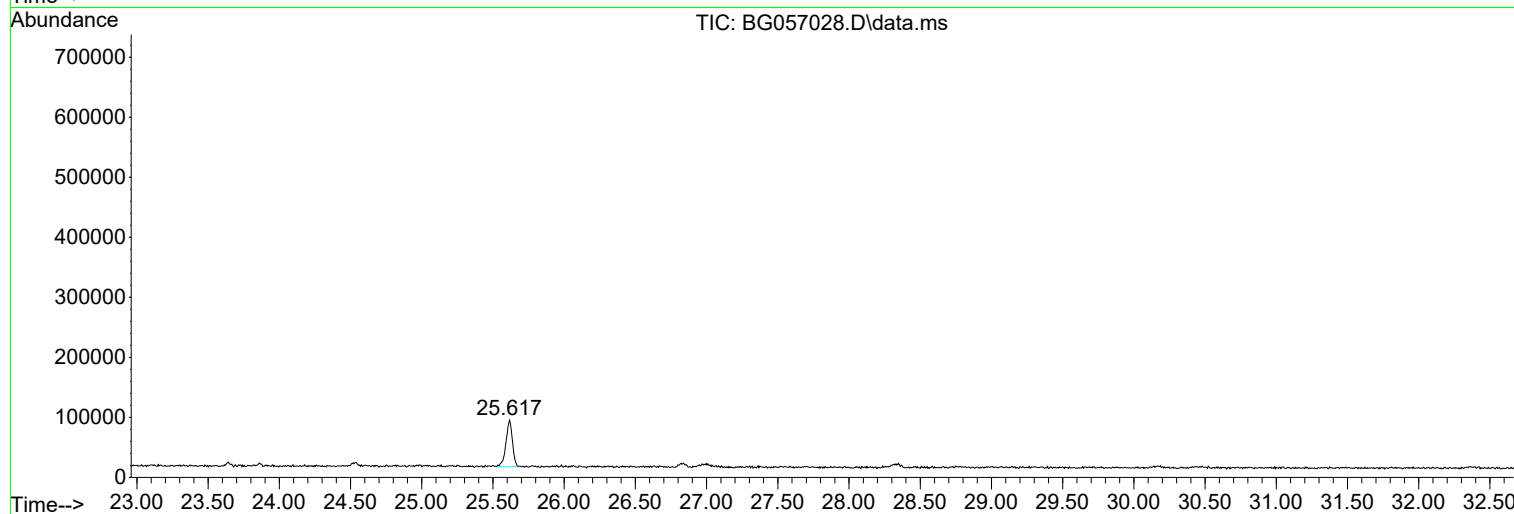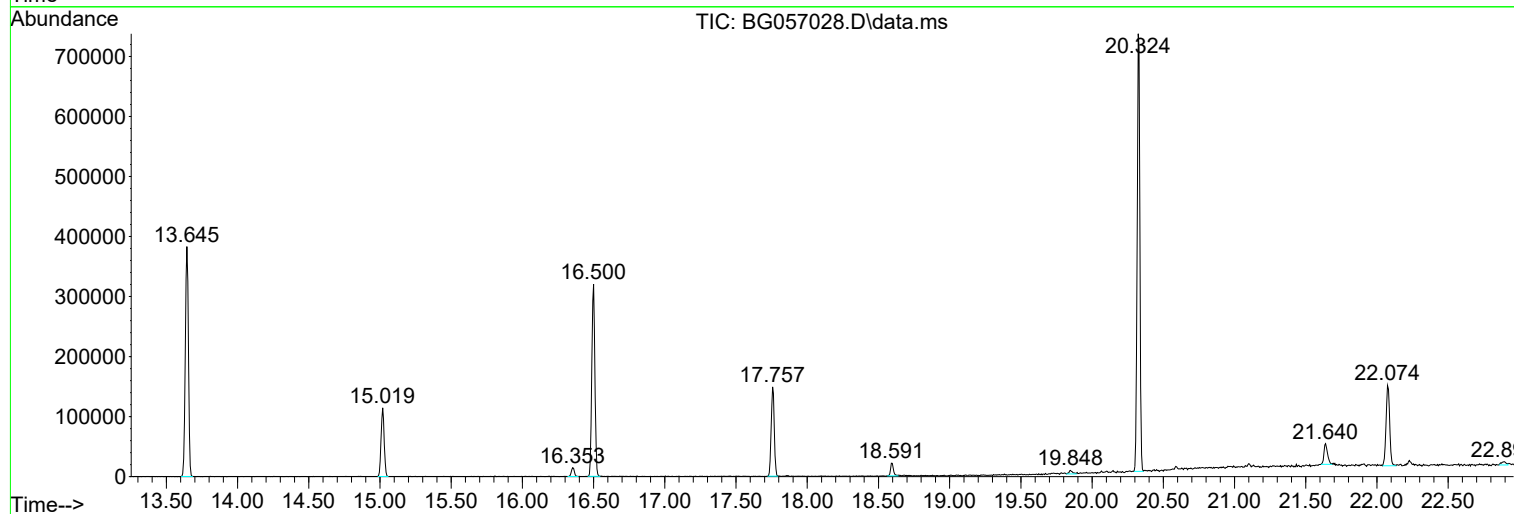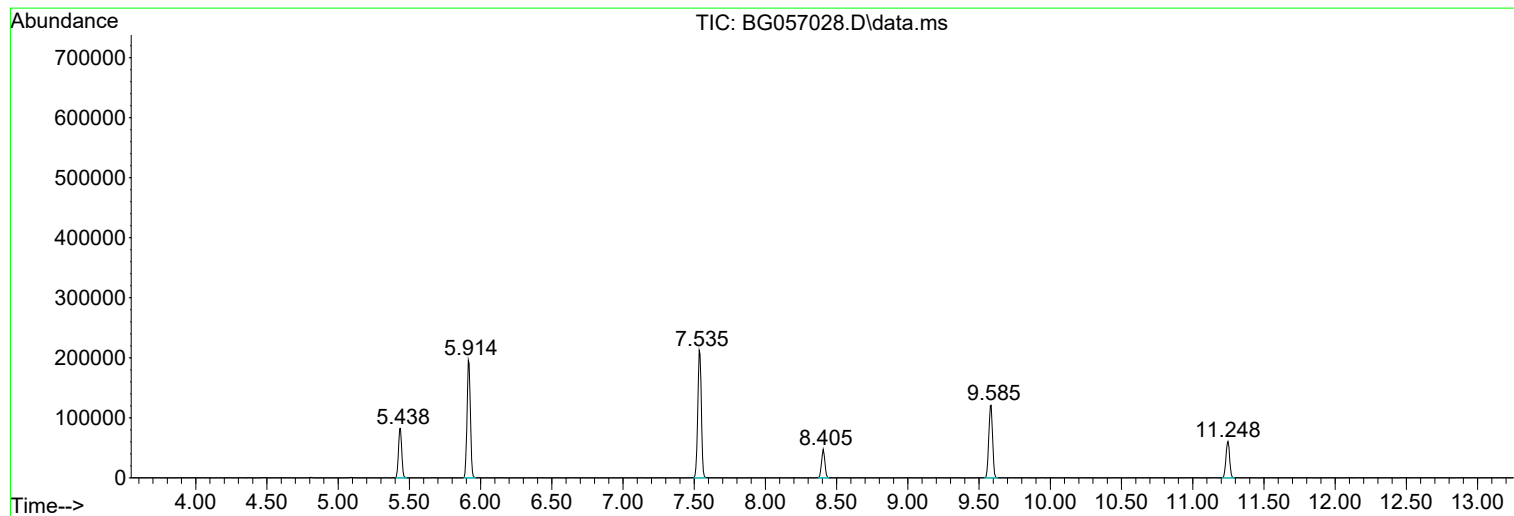

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057028.D
Acq On : 7 Apr 2023 15:58
Operator : CG/JU
Sample : 02224-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057028.D
Acq On : 7 Apr 2023 15:58
Operator : CG/JU
Sample : 02224-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------