

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
 Data File : BG057030.D
 Acq On : 7 Apr 2023 17:21
 Operator : CG/JU
 Sample : 02224-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU3-FC-BACKFILL-04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.430	317	322	330	rBB	75799	119149	13.08%	3.023%
2	5.911	398	404	413	rBB	175796	287796	31.58%	7.303%
3	7.539	673	681	688	rBB	189874	328905	36.09%	8.346%
4	8.408	823	829	835	rBB	42498	70060	7.69%	1.778%
5	9.583	1021	1029	1036	rBB	115387	204474	22.44%	5.188%
6	11.245	1305	1312	1322	rBB	60767	104643	11.48%	2.655%
7	13.648	1713	1721	1728	rBV	352083	534779	58.69%	13.569%
8	15.023	1948	1955	1963	rBB2	110778	170035	18.66%	4.314%
9	16.356	2178	2182	2187	rBV	10970	14268	1.57%	0.362%
10	16.503	2200	2207	2216	rVB	291244	452195	49.62%	11.474%
11	17.760	2415	2421	2429	rBV	152214	222612	24.43%	5.649%
12	18.594	2559	2563	2569	rBV2	14052	20404	2.24%	0.518%
13	20.327	2852	2858	2864	rBV	718984	911243	100.00%	23.122%
14	21.643	3077	3082	3091	rVB5	28887	57179	6.27%	1.451%
15	22.078	3150	3156	3162	rBV2	132435	226013	24.80%	5.735%
16	25.620	3750	3759	3769	rVB2	69761	217283	23.84%	5.513%




Sum of corrected areas: 3941038

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057030.D
Acq On : 7 Apr 2023 17:21
Operator : CG/JU
Sample : 02224-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

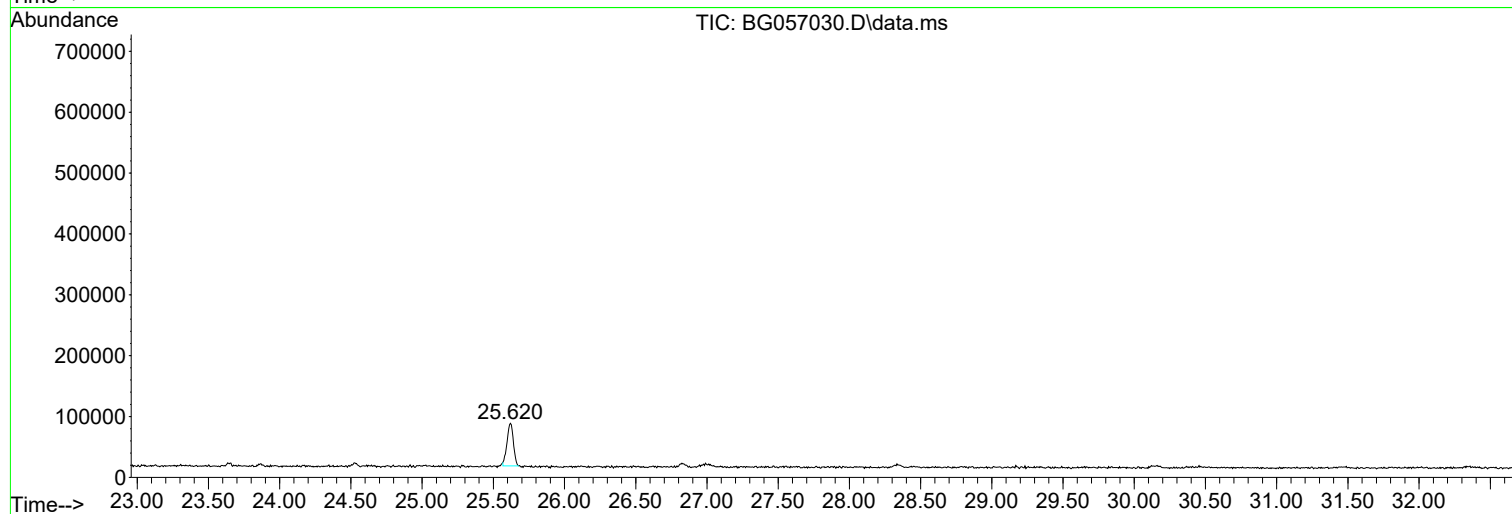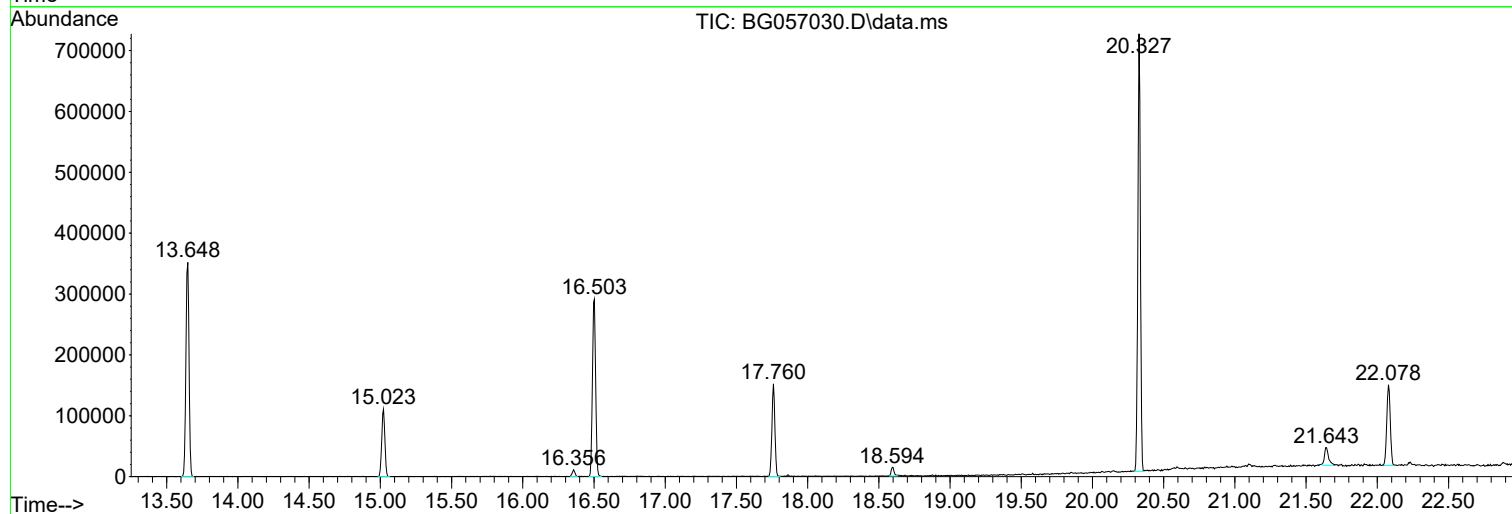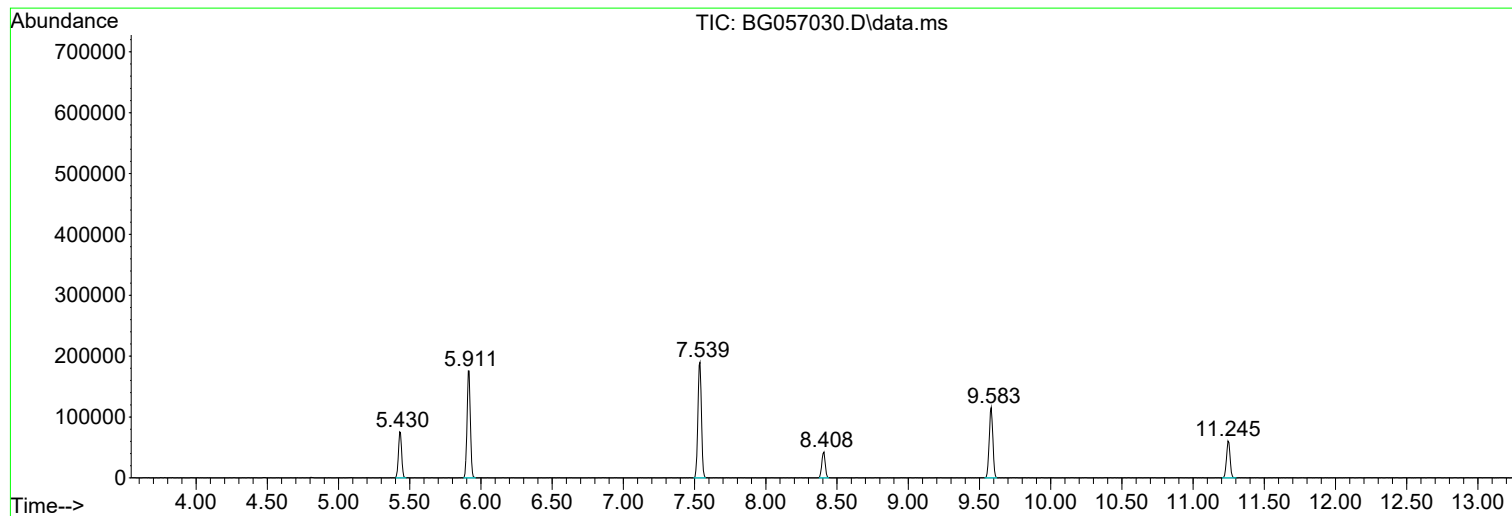

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057030.D
Acq On : 7 Apr 2023 17:21
Operator : CG/JU
Sample : 02224-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057030.D
Acq On : 7 Apr 2023 17:21
Operator : CG/JU
Sample : 02224-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------