

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
 Data File : BG057032.D
 Acq On : 7 Apr 2023 18:44
 Operator : CG/JU
 Sample : 02224-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU3-FC-BACKFILL-08

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.436	317	323	329	rBV	85861	132308	13.95%	3.177%
2	5.917	395	405	413	rBB	217208	345904	36.48%	8.306%
3	7.539	674	681	691	rBB	228143	382729	40.36%	9.190%
4	8.402	822	828	835	rBB2	44995	74548	7.86%	1.790%
5	9.583	1020	1029	1037	rBB	123189	227117	23.95%	5.454%
6	11.245	1305	1312	1319	rBB	59233	104697	11.04%	2.514%
7	13.642	1713	1720	1727	rBV	382259	574847	60.62%	13.803%
8	15.017	1948	1954	1960	rVB	105962	160793	16.96%	3.861%
9	16.350	2177	2181	2187	rVB2	13565	19107	2.01%	0.459%
10	16.497	2200	2206	2216	rBV	310808	459175	48.42%	11.026%
11	17.754	2414	2420	2426	rBV	134834	205965	21.72%	4.946%
12	18.588	2557	2562	2569	rBV5	11780	18128	1.91%	0.435%
13	20.321	2852	2857	2864	rBV	724672	948277	100.00%	22.770%
14	21.637	3077	3081	3093	rVB5	21831	42884	4.52%	1.030%
15	22.072	3149	3155	3162	rVB	128565	218642	23.06%	5.250%
16	22.783	3272	3276	3281	rVB7	6291	10956	1.16%	0.263%
17	23.852	3456	3458	3466	rVB8	7172	10290	1.09%	0.247%
18	25.614	3746	3758	3767	rVB3	70261	228229	24.07%	5.480%




Sum of corrected areas: 4164596

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057032.D
Acq On : 7 Apr 2023 18:44
Operator : CG/JU
Sample : 02224-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

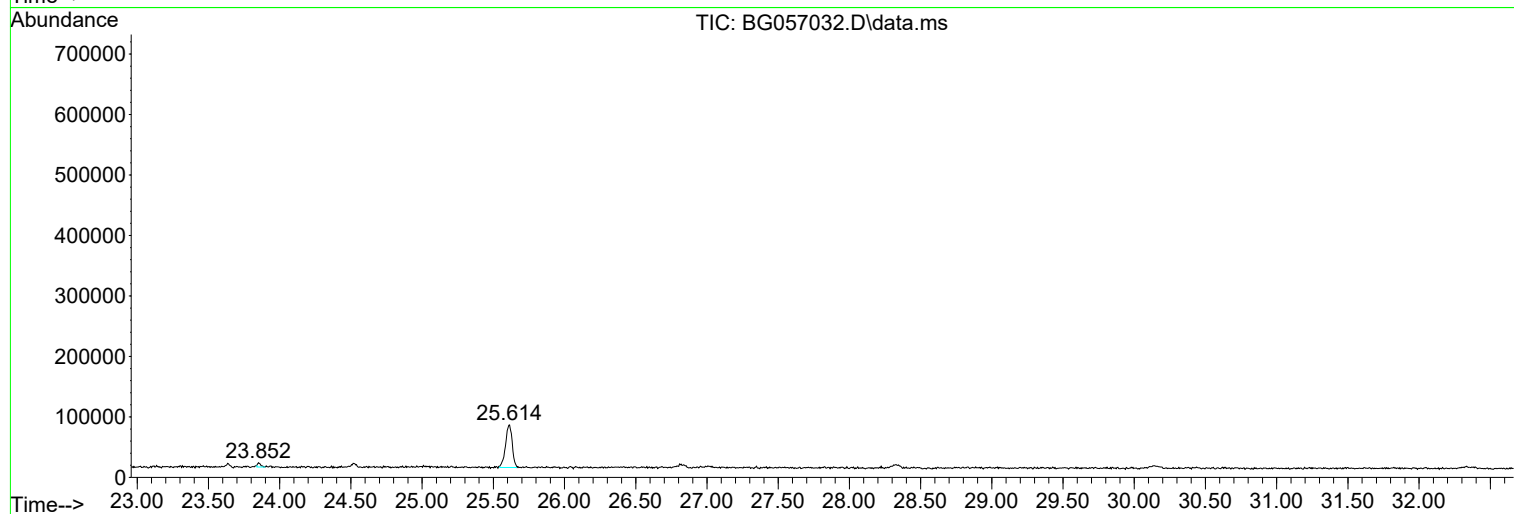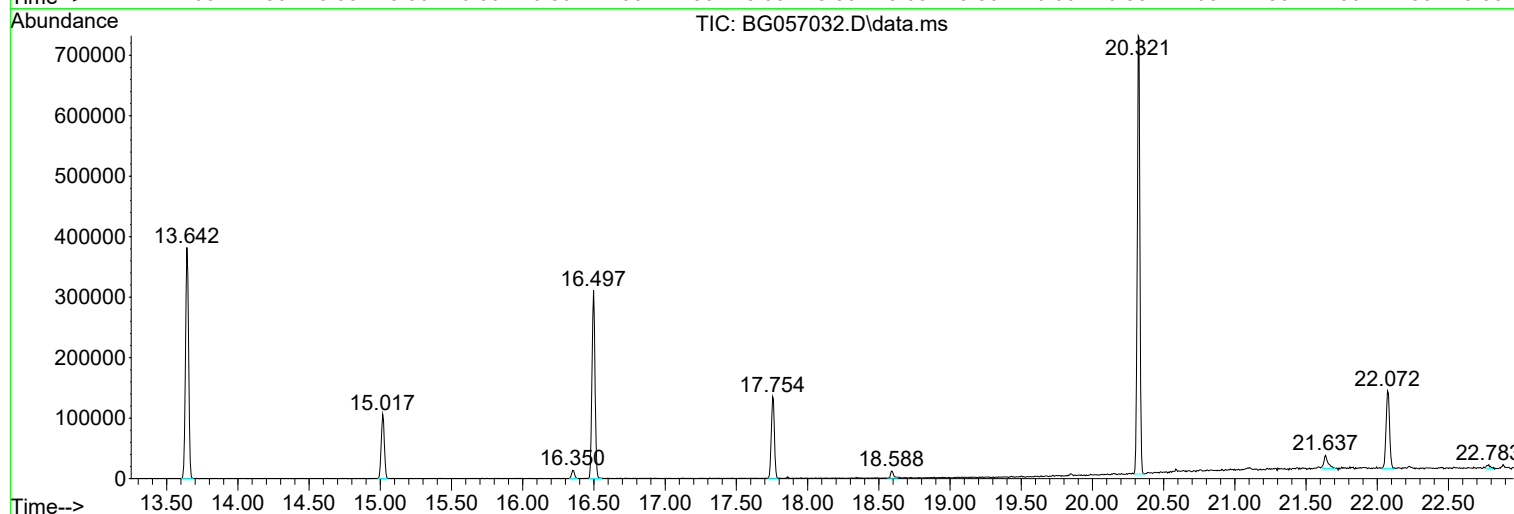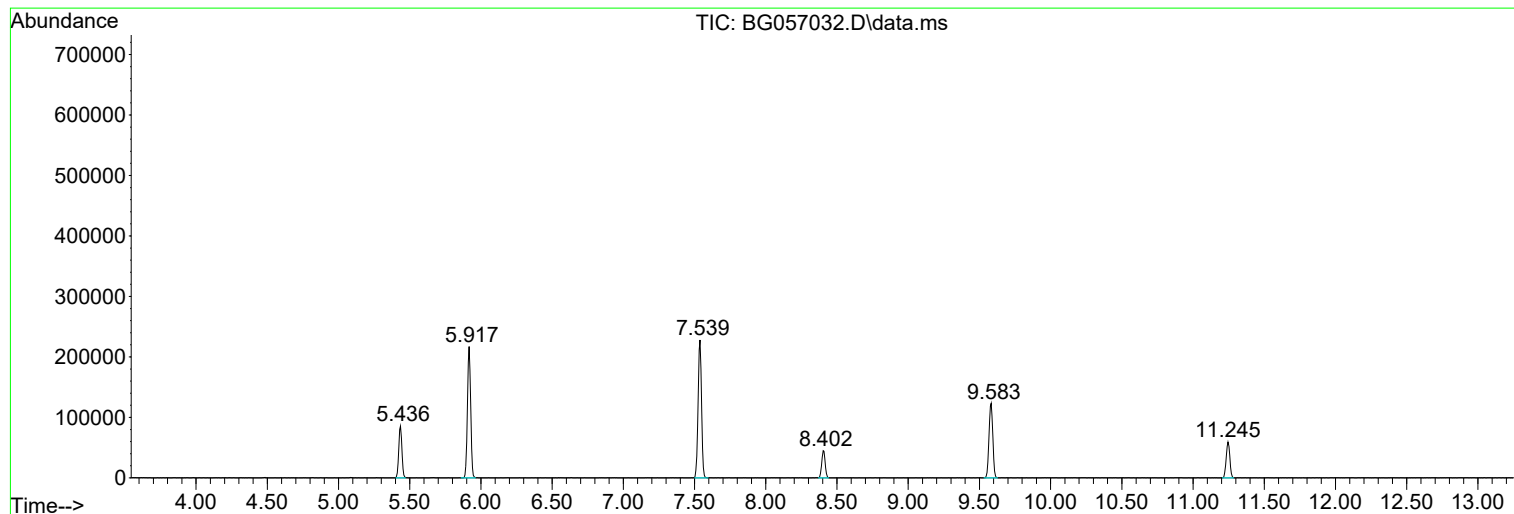

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057032.D
Acq On : 7 Apr 2023 18:44
Operator : CG/JU
Sample : 02224-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057032.D
Acq On : 7 Apr 2023 18:44
Operator : CG/JU
Sample : 02224-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-08

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------