

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
 Data File : BG057033.D
 Acq On : 7 Apr 2023 19:26
 Operator : CG/JU
 Sample : 02224-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU3-FC-BACKFILL-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.435	316	323	332	rBB	84415	127726	14.54%	3.218%
2	5.917	398	405	414	rBB	194927	317760	36.17%	8.005%
3	7.538	673	681	689	rBV	209275	363165	41.34%	9.149%
4	8.402	822	828	835	rBB	45941	77172	8.78%	1.944%
5	9.582	1021	1029	1036	rBB	126537	220749	25.13%	5.561%
6	11.245	1305	1312	1319	rBV	62600	110831	12.62%	2.792%
7	13.642	1714	1720	1731	rVB	368957	553747	63.03%	13.950%
8	15.016	1947	1954	1961	rVB3	109629	169329	19.27%	4.266%
9	16.350	2175	2181	2186	rBV	17743	24366	2.77%	0.614%
10	16.497	2200	2206	2213	rBV	283357	432742	49.26%	10.902%
11	17.754	2414	2420	2428	rBV	137824	213347	24.29%	5.375%
12	18.594	2559	2563	2569	rVB4	7306	9712	1.11%	0.245%
13	20.327	2852	2858	2864	rBV	690331	878510	100.00%	22.132%
14	21.637	3077	3081	3088	rBV4	23445	35921	4.09%	0.905%
15	22.071	3149	3155	3161	rBV	125191	211935	24.12%	5.339%
16	25.614	3744	3758	3767	rBV	70616	222469	25.32%	5.604%




Sum of corrected areas: 3969481

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057033.D
Acq On : 7 Apr 2023 19:26
Operator : CG/JU
Sample : 02224-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

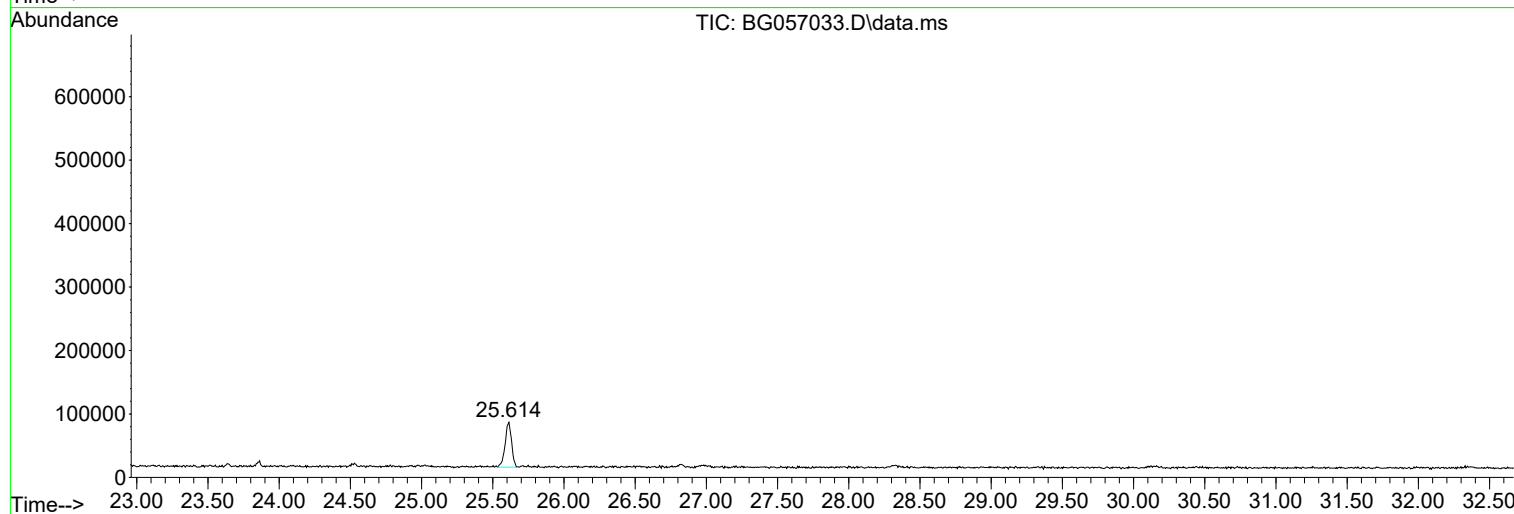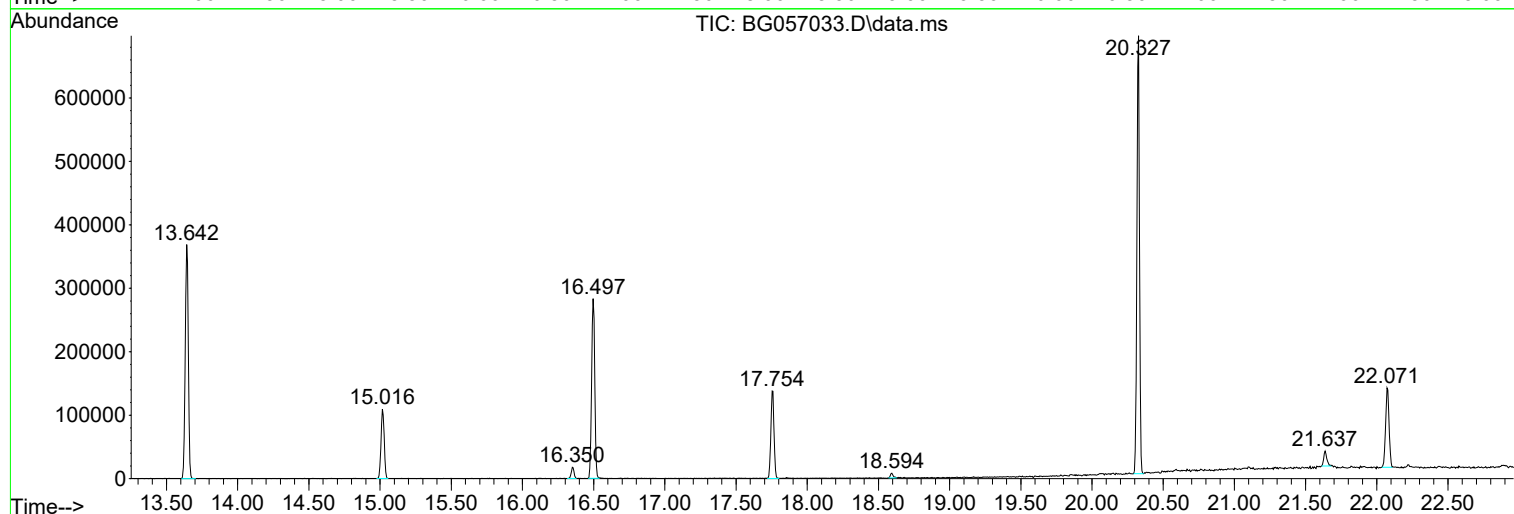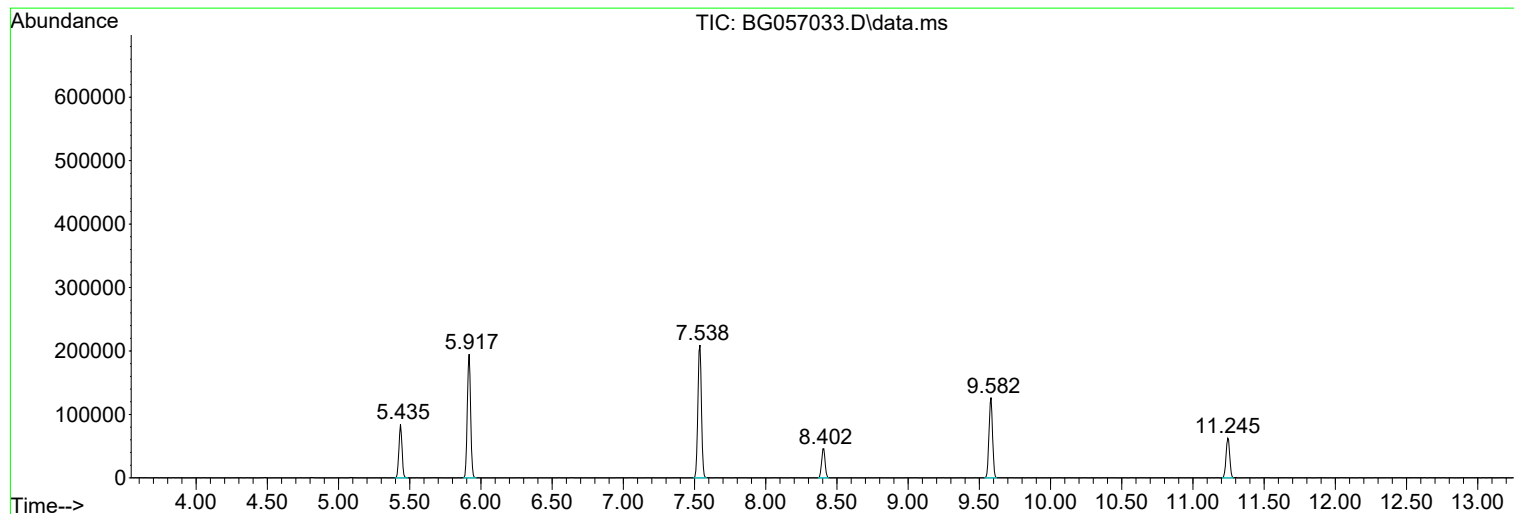

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057033.D
Acq On : 7 Apr 2023 19:26
Operator : CG/JU
Sample : 02224-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057033.D
Acq On : 7 Apr 2023 19:26
Operator : CG/JU
Sample : 02224-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------