

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
 Data File : BG057034.D
 Acq On : 7 Apr 2023 20:07
 Operator : CG/JU
 Sample : 02224-21
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU3-FC-BACKFILL-11

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG057034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.436	317	323	330	rBB	73225	113615	14.96%	3.296%
2	5.917	398	405	413	rBB	143722	234446	30.87%	6.802%
3	7.533	672	680	690	rBB	174835	300859	39.62%	8.729%
4	8.402	822	828	836	rBB	46101	77198	10.17%	2.240%
5	9.577	1021	1028	1036	rBB	103925	193038	25.42%	5.600%
6	11.245	1305	1312	1321	rBB	64663	110206	14.51%	3.197%
7	13.642	1714	1720	1727	rVB	332233	489690	64.48%	14.207%
8	15.017	1948	1954	1961	rVB2	108794	168959	22.25%	4.902%
9	16.350	2174	2181	2186	rVB2	18410	26393	3.48%	0.766%
10	16.497	2199	2206	2214	rBV	154005	228716	30.12%	6.636%
11	17.754	2413	2420	2428	rBV	140686	212582	27.99%	6.167%
12	20.321	2852	2857	2863	rVB	600962	759436	100.00%	22.033%
13	21.637	3077	3081	3095	rVB4	26728	50445	6.64%	1.464%
14	22.072	3149	3155	3162	rBV2	121315	215779	28.41%	6.260%
15	22.225	3176	3181	3186	rBV8	5598	10680	1.41%	0.310%
16	23.852	3452	3458	3463	rBV6	9394	20432	2.69%	0.593%
17	24.521	3570	3572	3579	rVB8	7374	11162	1.47%	0.324%
18	25.608	3748	3757	3769	rVB3	69357	223215	29.39%	6.476%




Sum of corrected areas: 3446851

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057034.D
Acq On : 7 Apr 2023 20:07
Operator : CG/JU
Sample : 02224-21
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

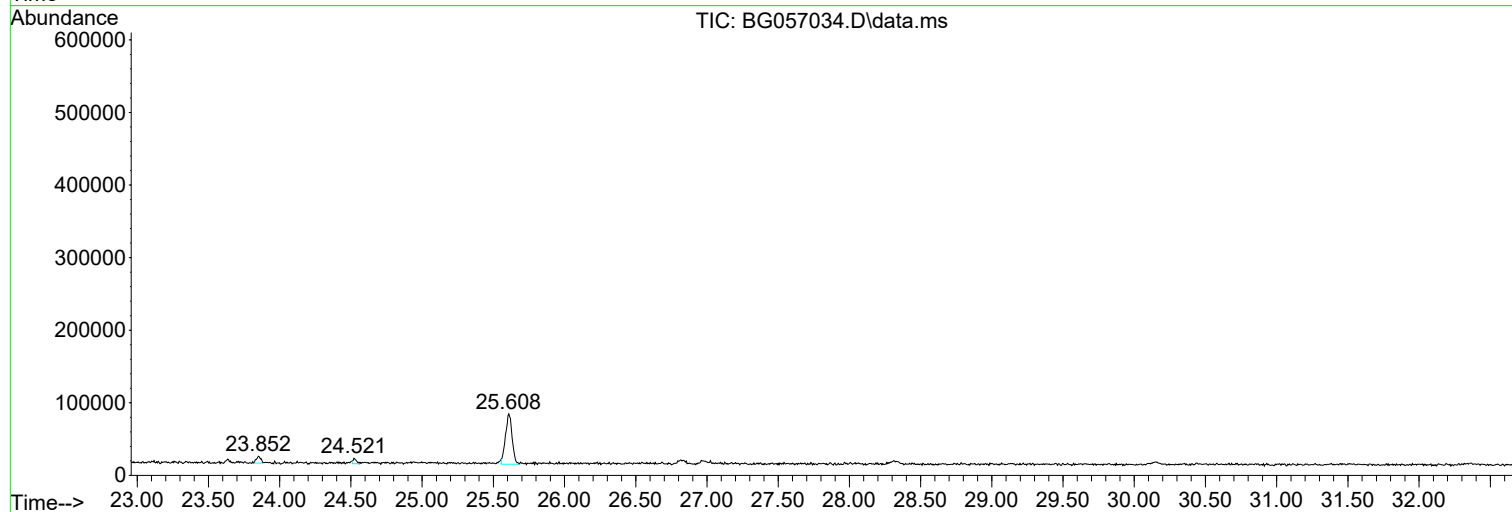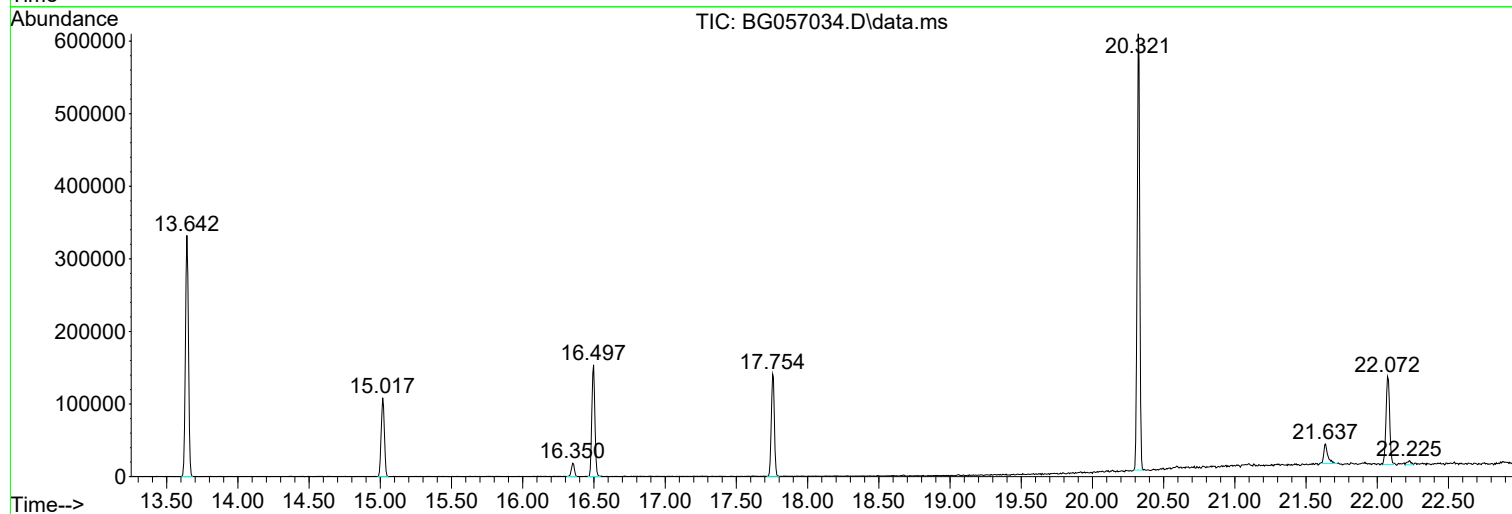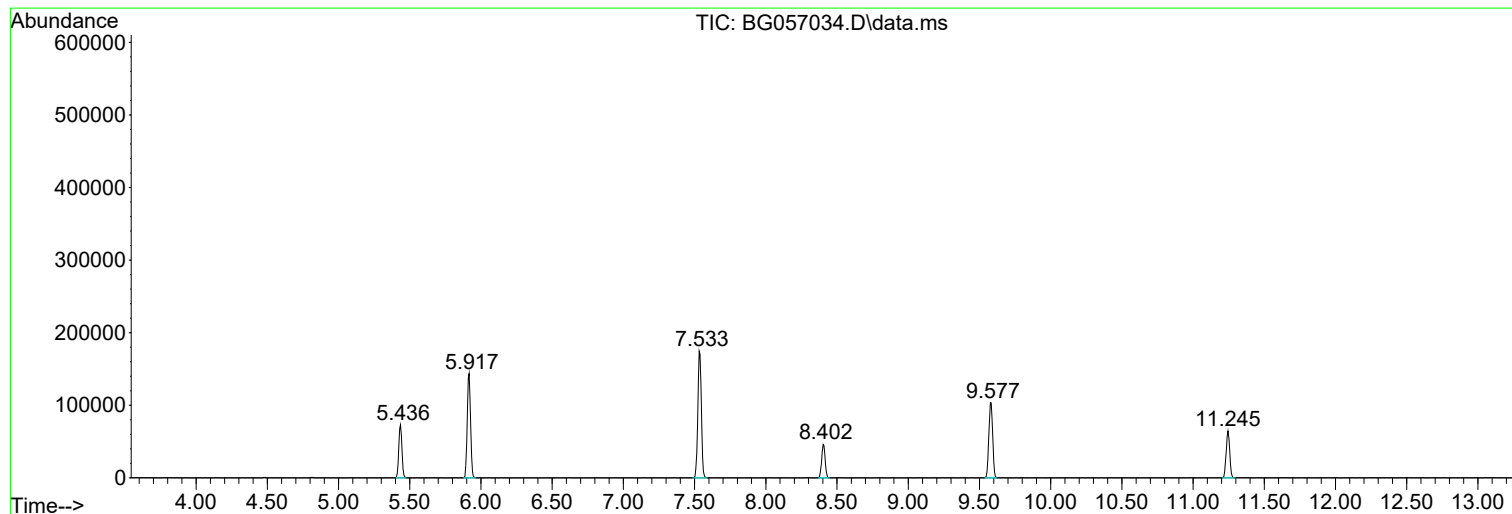

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057034.D
Acq On : 7 Apr 2023 20:07
Operator : CG/JU
Sample : 02224-21
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057034.D
Acq On : 7 Apr 2023 20:07
Operator : CG/JU
Sample : 02224-21
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU3-FC-BACKFILL-11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------