


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057021.D
Acq On : 7 Apr 2023 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Apr 08 04:45:47 2023

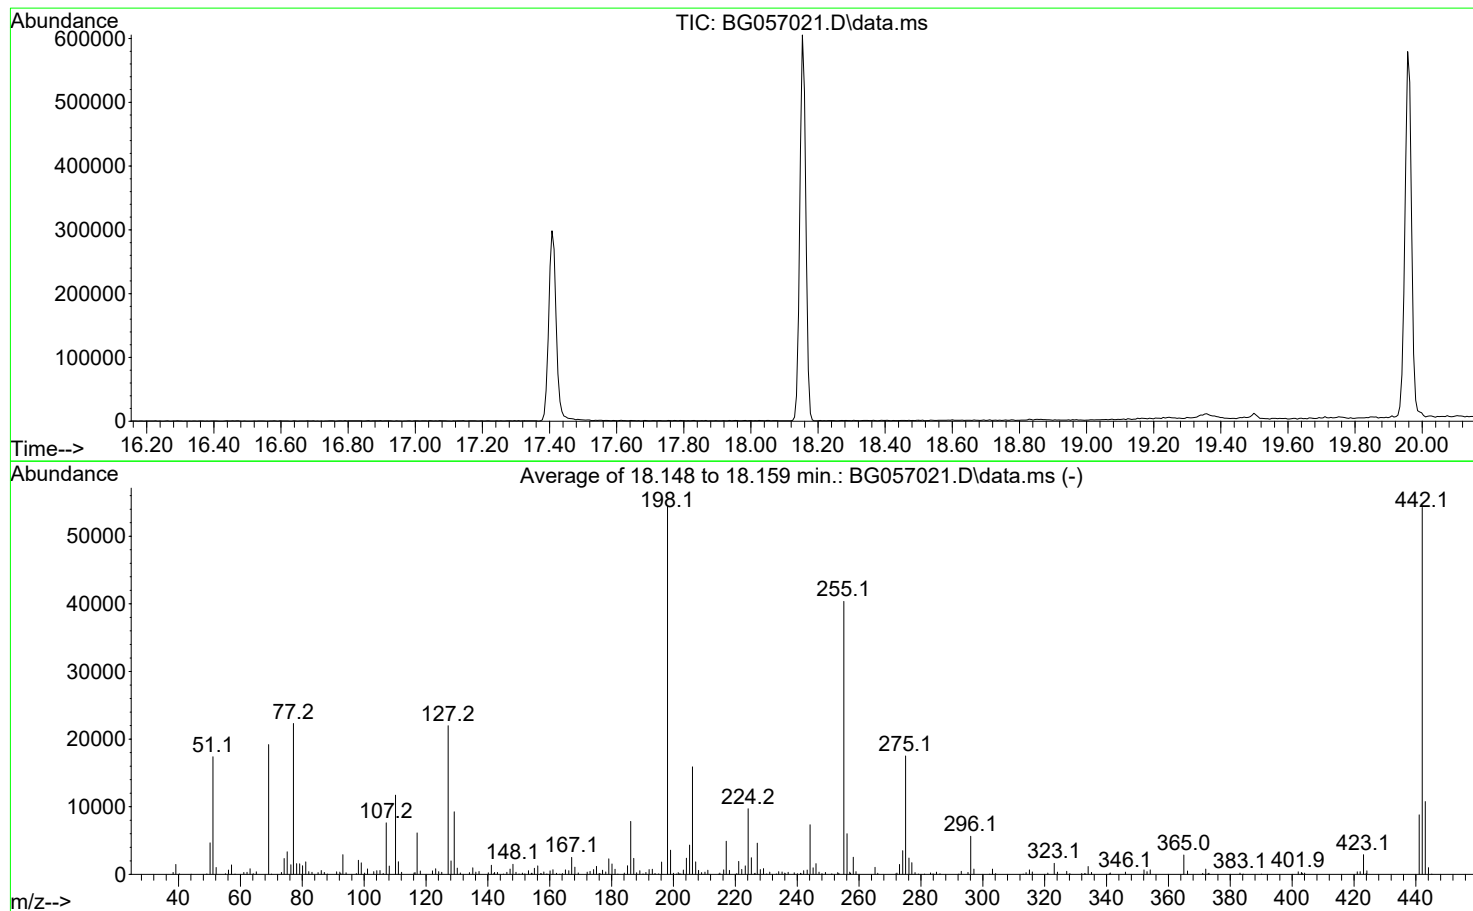

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	17385	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.3	19195	PASS
70	69	0.00	2	0.3	53	PASS
127	198	10	80	40.4	21987	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54397	PASS
199	198	5	9	6.6	3580	PASS
275	198	10	60	32.2	17500	PASS
365	198	1	100	5.2	2853	PASS
441	198	0.01	100	16.2	8814	PASS
442	442	50	100	100.0	54253	PASS
443	442	15	24	19.8	10759	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/7/2023	BNA_G	BG057021.D
Compound Name	Response	Retention Time
DDT	156328	21.202
DDD	3514	20.732
DDE	121	20.239
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3635	159963	2.27

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057021.D
Acq On : 7 Apr 2023 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 08 05:05:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 04:45:47 2023
Response via : Initial Calibration

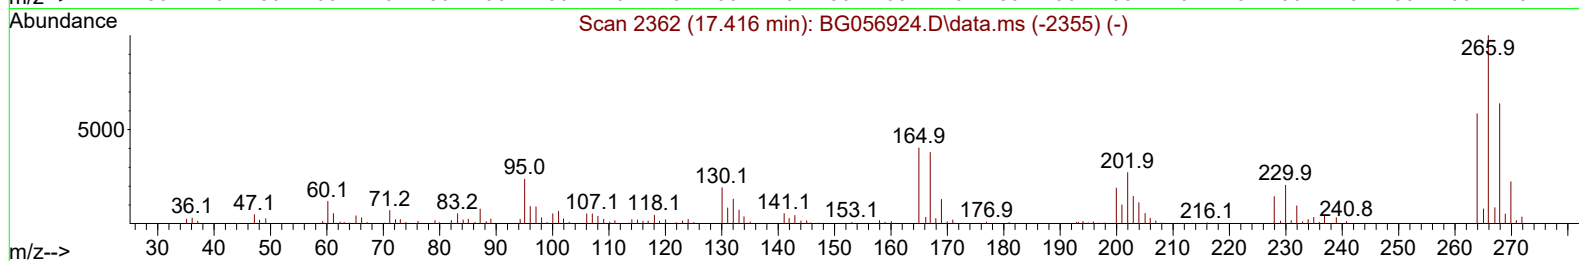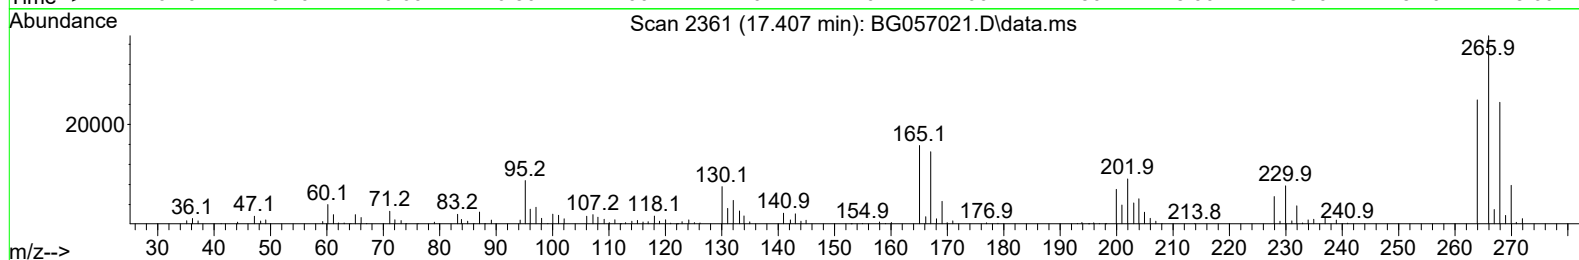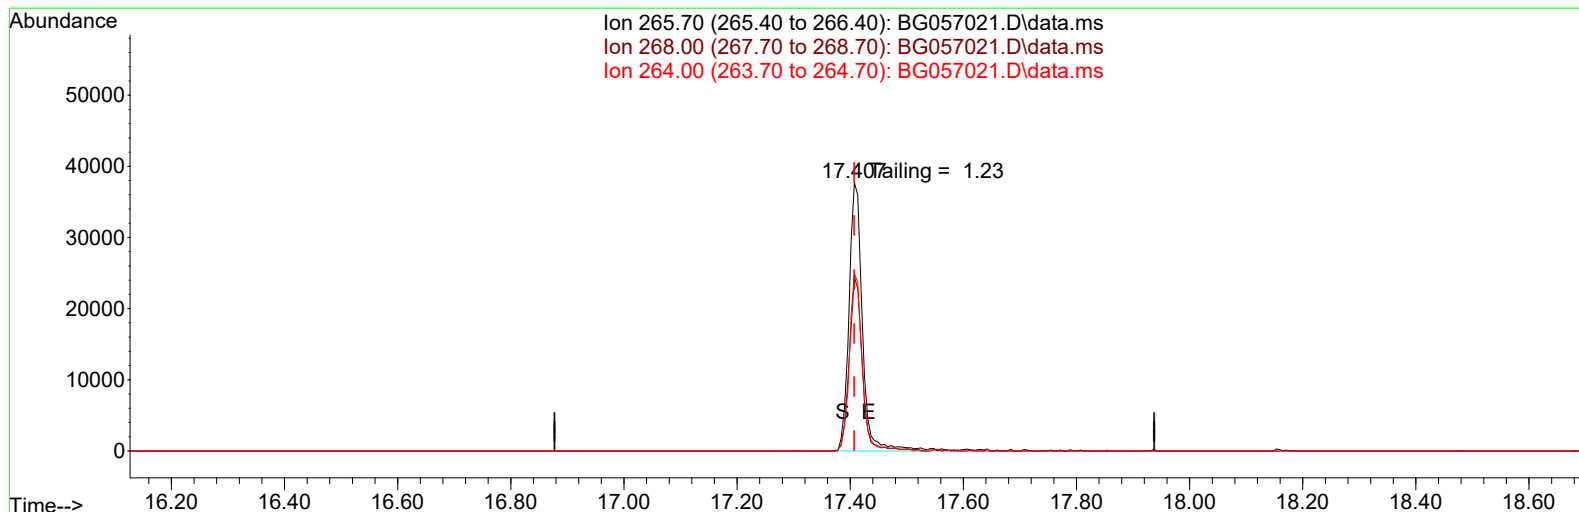

TIC: BG057021.D\data.ms

(70) Pentachlorophenol (C)

17.407min (+ 0.000) 29440.12 ng




response 62008

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.78
264.00	58.50	65.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040723\
Data File : BG057021.D
Acq On : 7 Apr 2023 10:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 08 05:05:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 04:45:47 2023
Response via : Initial Calibration

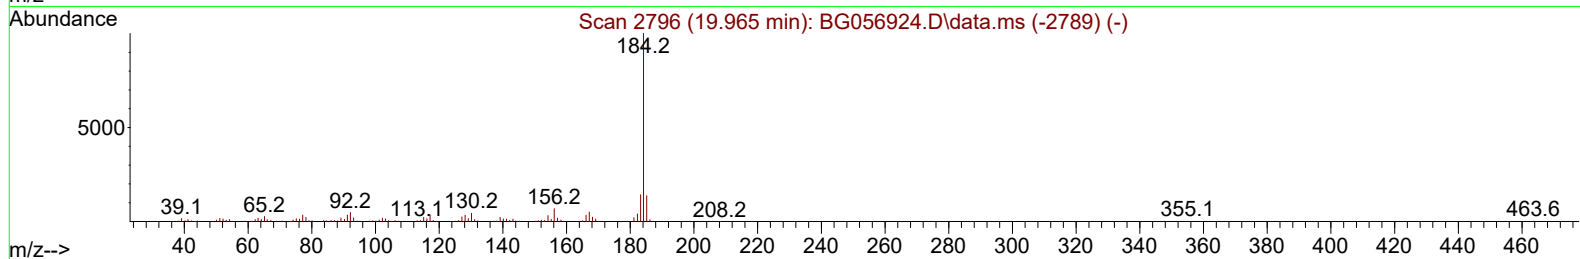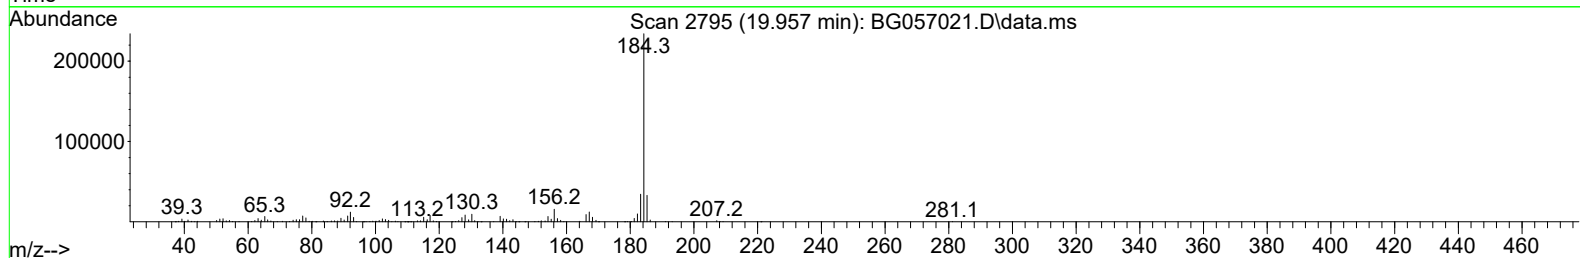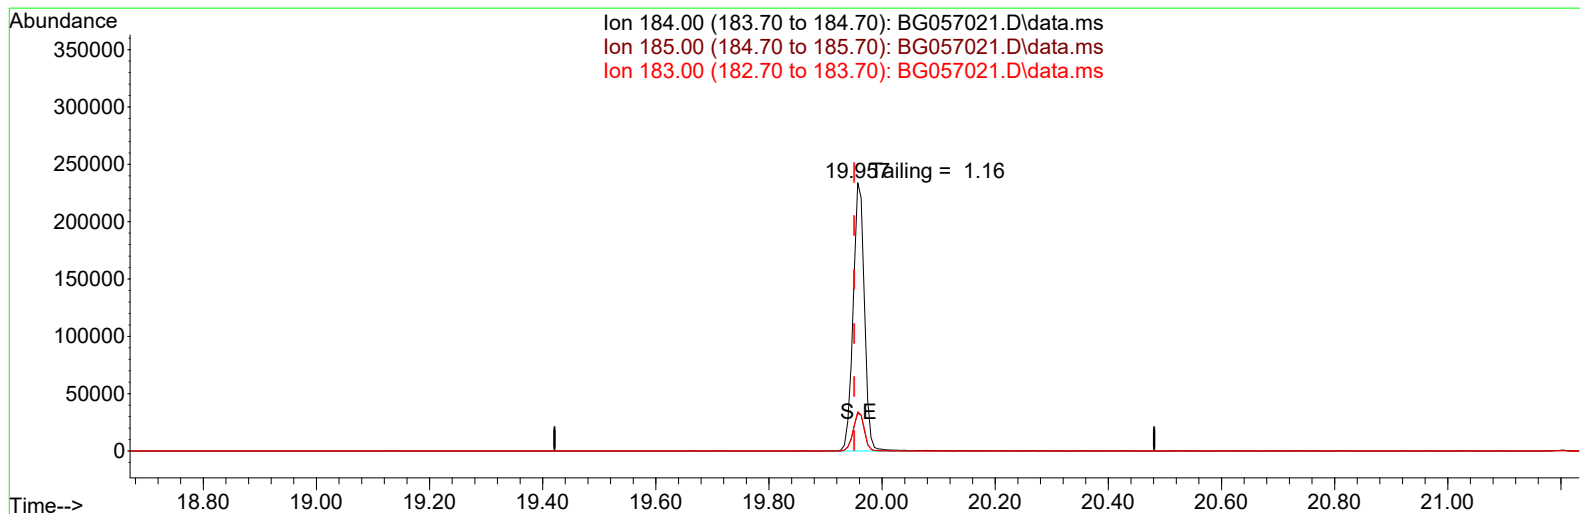

TIC: BG057021.D\data.ms

(77) Benzidine

19.957min (+ 0.006) 0.00 ng m

response 324614

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.13
183.00	14.20	14.70
0.00	0.00	0.00