
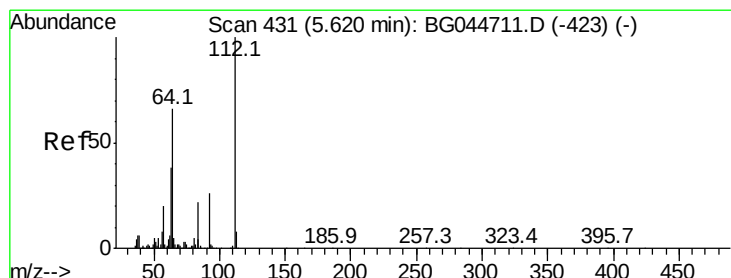
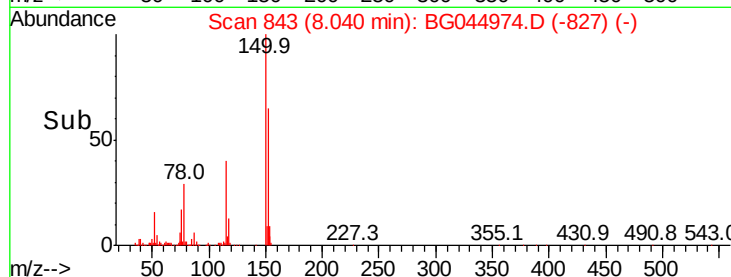
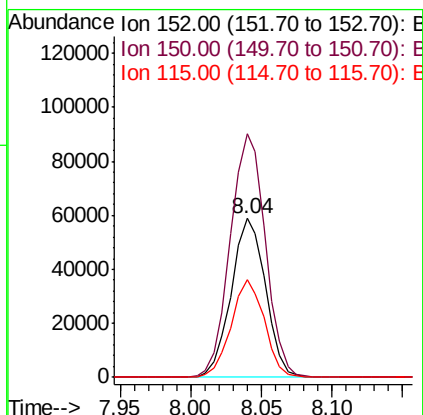


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 843
Delta R.T. -0.00 min
Lab File: BG044974.D
Acq: 8 Apr 2020 13:19

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	153.1	128.8	193.2
115	61.4	52.6	79.0

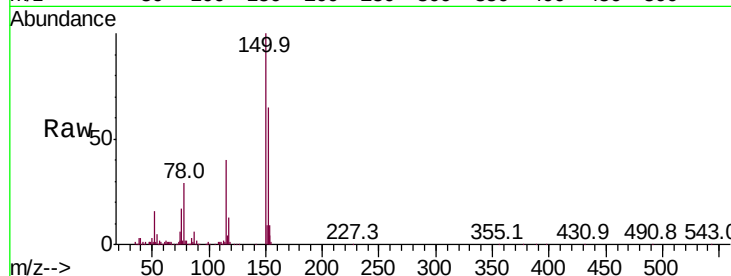

#5

2-Fluorophenol
Concen: 31.506 ng
RT: 5.61 min Scan# 430
Delta R.T. 0.00 min
Lab File: BG044974.D
Acq: 8 Apr 2020 13:19

Tgt Ion	Ratio	Lower	Upper
112	100		
64	56.7	53.4	80.2
63	31.4	29.4	44.2

