

#45

2-Fluorobiphenyl

Concen: 23.189 ng

RT: 13.29 min Scan# 1737

Delta R.T. -0.01 min

Lab File: BG044974.D

Acq: 8 Apr 2020 13:19

Instrument :

BNA_G

ClientSampleId :


Tot Ion:172 Resp: 426252

Ion	Ratio	Lower	Upper
172	100		
171	37.1	28.7	43.1
170	22.9	19.0	28.6

172 100

171 37.1 28.7 43.1




170 22.9 19.0 28.6

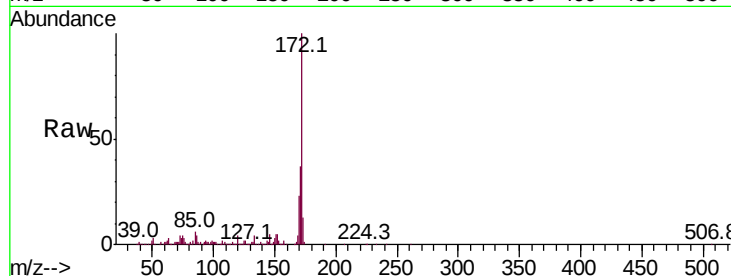

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

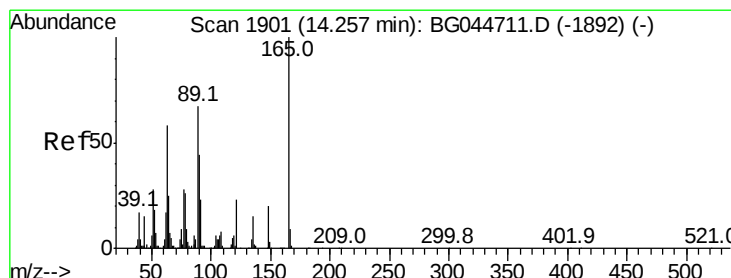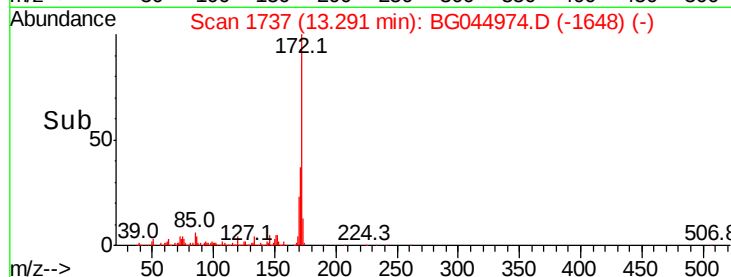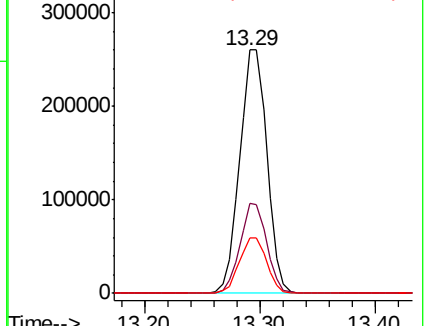

#51

2,6-Dinitrotoluene

Concen: 8.169 ng

RT: 14.67 min Scan# 1972

Delta R.T. 0.43 min

Lab File: BG044974.D

Acq: 8 Apr 2020 13:19


Tgt Ion:165 Resp: 34523

Ion	Ratio	Lower	Upper
165	100		
63	2.3	45.8	68.8#
89	2.5	51.8	77.6#

165 100

63 2.3 45.8 68.8#

89 2.5 51.8 77.6#

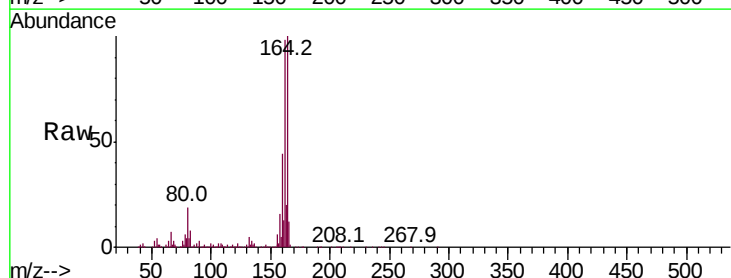

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

