

#75

Fluoranthene

Concen: 32.643 ng

RT: 19.47 min Scan# 2789

Delta R.T. 0.00 min

Lab File: BG044974.D

Acq: 8 Apr 2020 13:19


Instrument :

BNA_G

ClientSampleId :

Tot Ion:202 Resp: 1076374




Ion	Ratio	Lower	Upper
202	100		
101	8.6	0.0	29.8
203	19.5	0.0	39.4

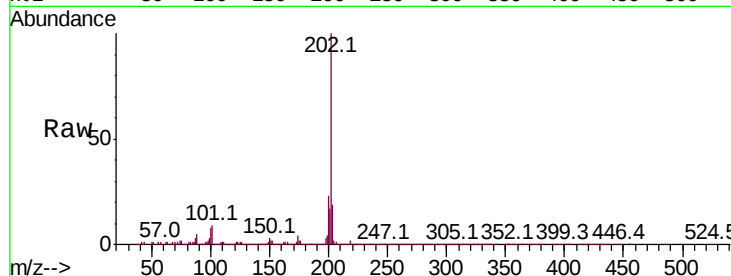

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

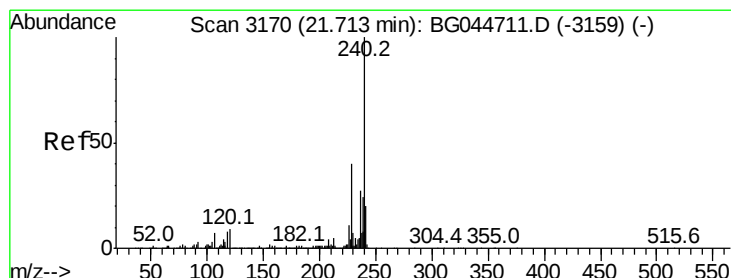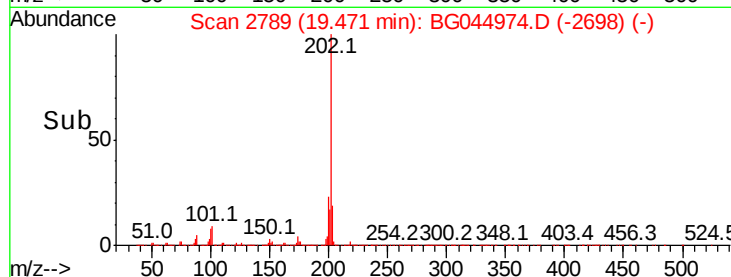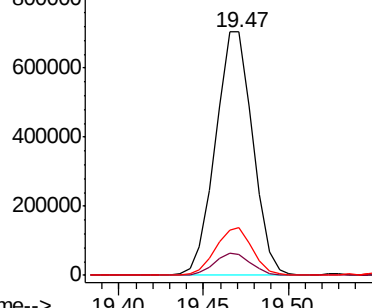

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3166


Delta R.T. -0.00 min

Lab File: BG044974.D

Acq: 8 Apr 2020 13:19

Tgt Ion:240 Resp: 432994

Ion	Ratio	Lower	Upper
240	100		
120	8.4	6.7	10.1
236	25.4	21.5	32.3

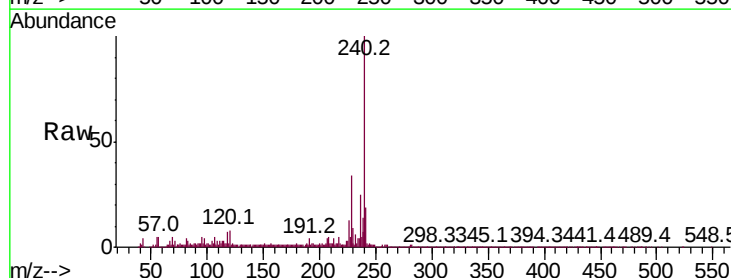

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

