

#81

Benzo(a)anthracene

Concen: 19.336 ng

RT: 21.67 min Scan# 3163

Delta R.T. -0.00 min

Lab File: BG044974.D

Acq: 8 Apr 2020 13:19

Instrument :

BNA_G

ClientSampleId :


Tot Ion:228 Resp: 602858

Ion Ratio Lower Upper




228 100

226 29.9 23.6 35.4

229 22.4 17.1 25.7

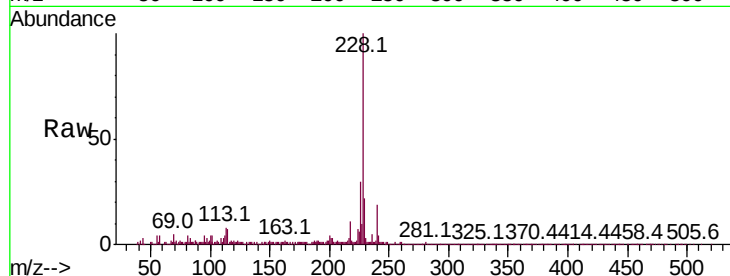

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

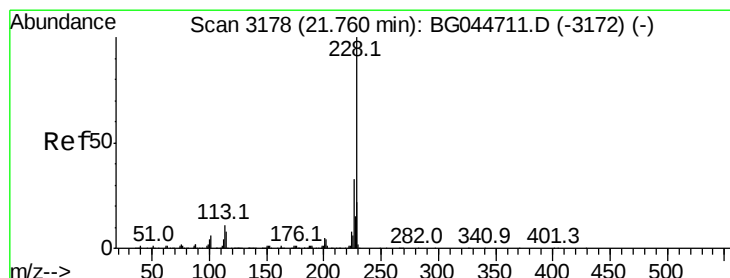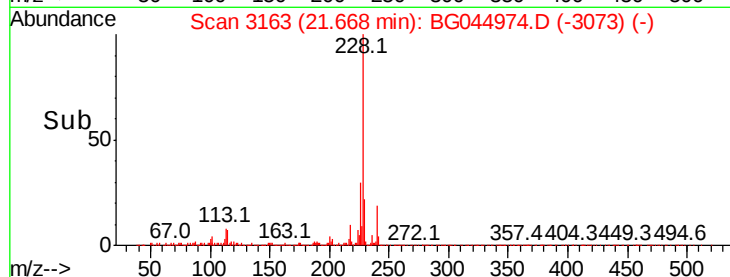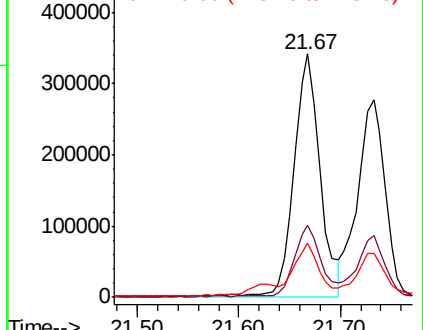

#83

Chrysene

Concen: 17.463 ng

RT: 21.73 min Scan# 3174

Delta R.T. -0.00 min

Lab File: BG044974.D

Acq: 8 Apr 2020 13:19


Tgt Ion:228 Resp: 520100

Ion Ratio Lower Upper

228 100

226 31.6 25.9 38.9

229 22.2 17.4 26.0

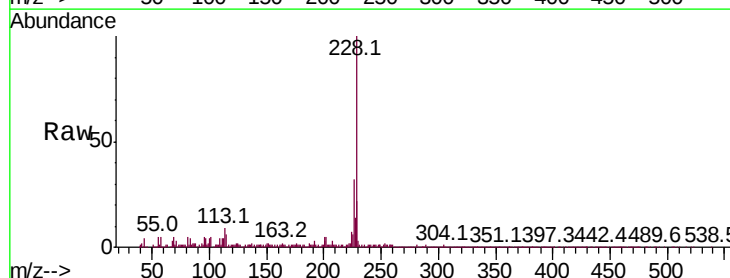

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

