

#90

Benzo(a)pyrene

Concen: 18.224 ng

RT: 24.73 min Scan# 3685

Delta R.T. -0.01 min

Lab File: BG044974.D

Acq: 8 Apr 2020 13:19

Instrument :

BNA_G

ClientSampleId :


Tot Ion:252 Resp: 550926

Ion Ratio Lower Upper

252 100

253 24.2 19.4 29.0




125 8.9 7.2 10.8

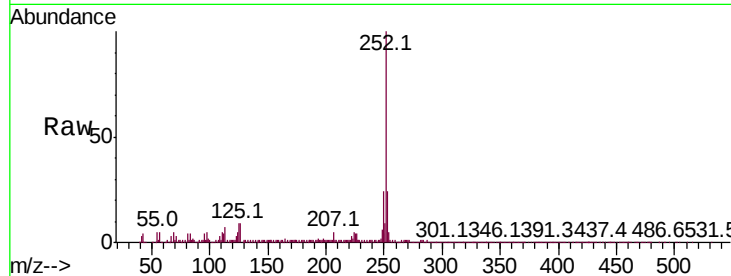

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

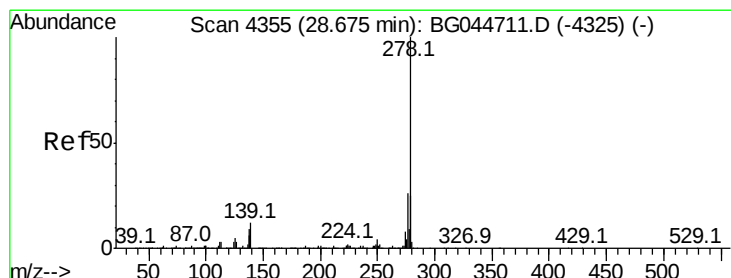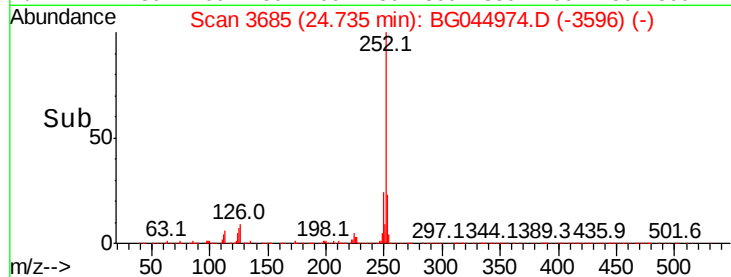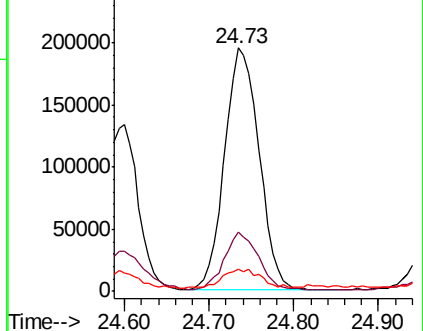

#91

Dibenzo(a,h)anthracene

Concen: 3.079 ng

RT: 28.56 min Scan# 4337

Delta R.T. -0.04 min

Lab File: BG044974.D

Acq: 8 Apr 2020 13:19


Tgt Ion:278 Resp: 91837

Ion Ratio Lower Upper

278 100

139 14.0 10.2 15.2

279 27.2 18.9 28.3

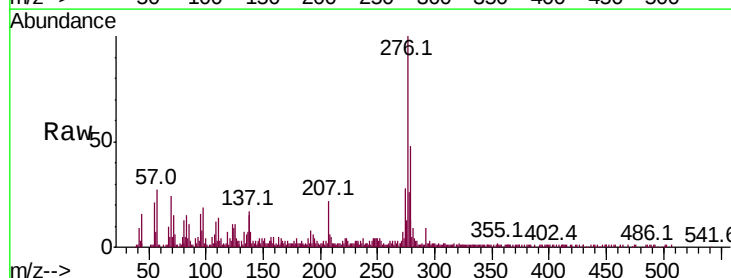

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

