


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 842
Delta R.T. -0.01 min
Lab File: BG044975.D
Acq: 8 Apr 2020 13:59

Instrument :
BNA_G
ClientSampled :

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.1	128.8	193.2
115	54.5	52.6	79.0

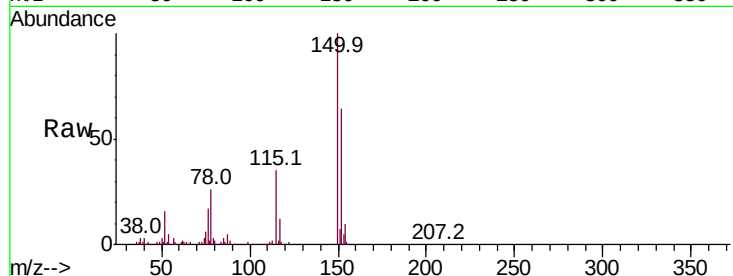


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

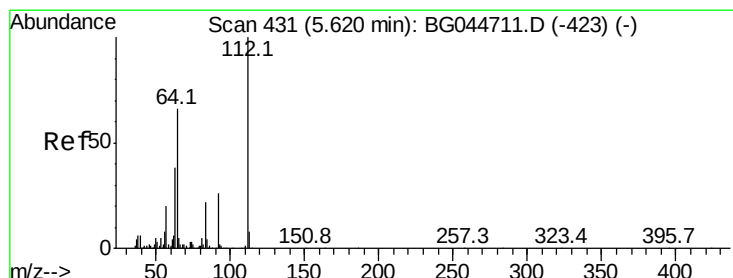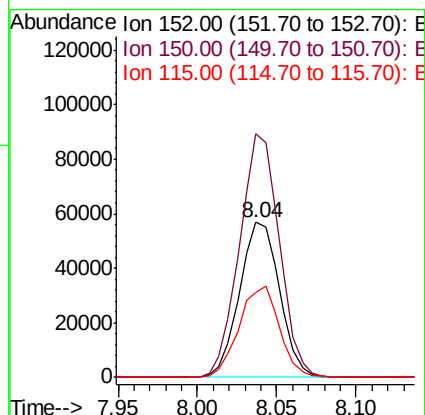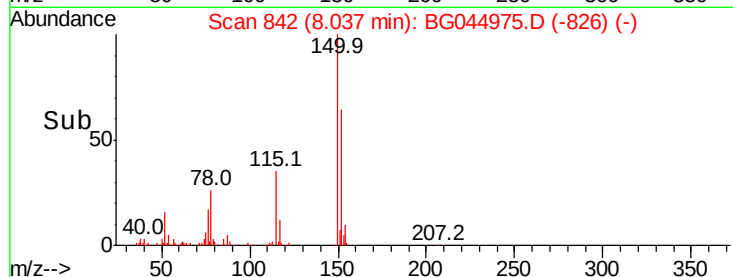

#5

2-Fluorophenol
Concen: 31.693 ng
RT: 5.61 min Scan# 429
Delta R.T. -0.00 min
Lab File: BG044975.D
Acq: 8 Apr 2020 13:59

Tgt Ion	Ratio	Lower	Upper
112	100		
64	52.4	53.4	80.2#
63	31.5	29.4	44.2

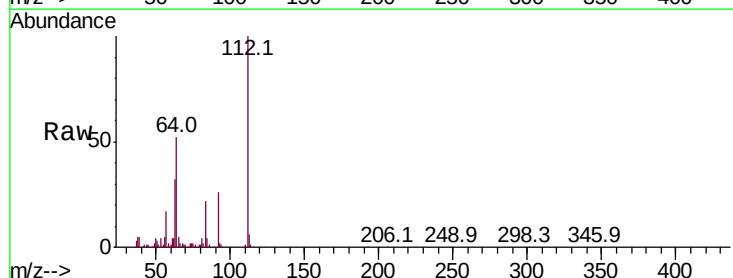

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

