
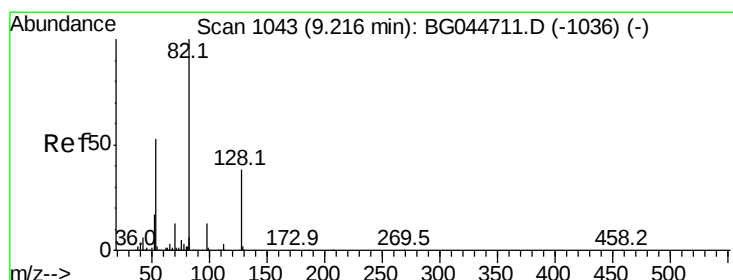
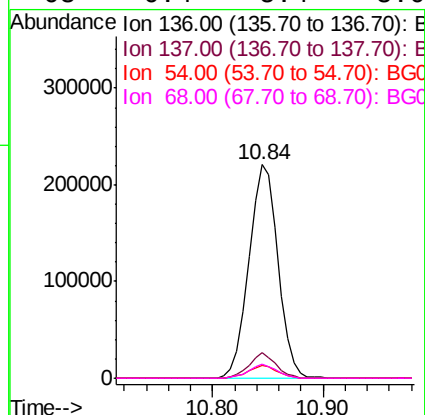
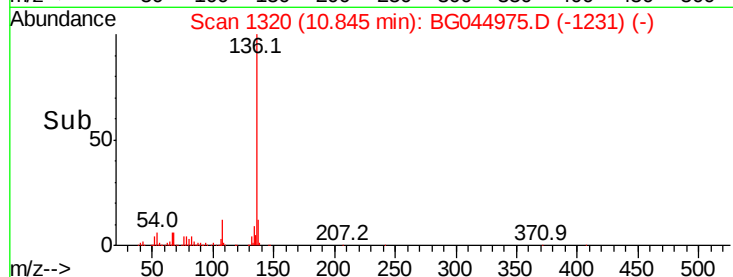


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.84 min Scan# 1320
Delta R.T. -0.01 min
Lab File: BG044975.D
Acq: 8 Apr 2020 13:59

Instrument :
BNA_G
ClientSampleId :

Tot Ion:136	Resp:	407552
Ion	Ratio	Lower Upper
136	100	
137	11.7	9.8 14.6
54	6.3	7.9 11.9#
68	6.4	5.4 8.0

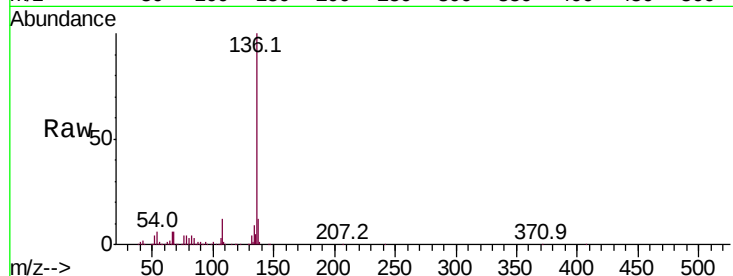

#23
Nitrobenzene-d5
Concen: 21.485 ng
RT: 9.19 min Scan# 1039
Delta R.T. -0.01 min
Lab File: BG044975.D
Acq: 8 Apr 2020 13:59

Tgt Ion: 82	Resp:	199545
Ion	Ratio	Lower Upper
82	100	
128	39.9	30.6 46.0
54	39.2	37.1 55.7

