
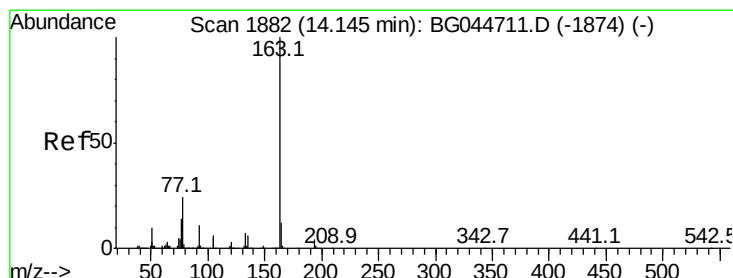
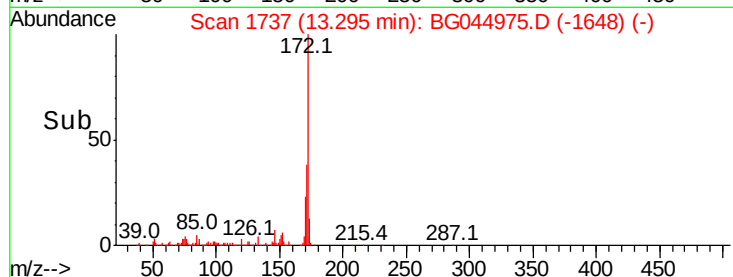
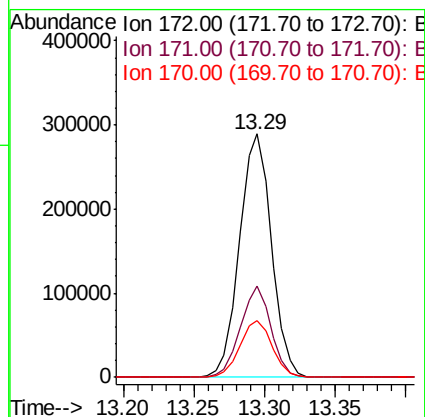


#45
 2-Fluorobiphenyl
 Concen: 23.334 ng
 RT: 13.29 min Scan# 1737
 Delta R.T. -0.01 min
 Lab File: BG044975.D
 Acq: 8 Apr 2020 13:59

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
172	100		
171	37.6	28.7	43.1
170	23.3	19.0	28.6

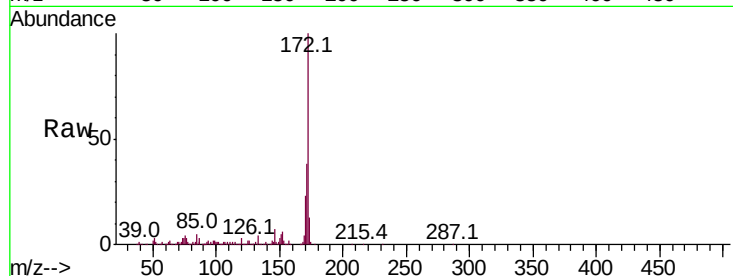

#50
 Dimethylphthalate
 Concen: 2.406 ng
 RT: 14.12 min Scan# 1877
 Delta R.T. -0.01 min
 Lab File: BG044975.D
 Acq: 8 Apr 2020 13:59

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.9	3.7	5.5
164	11.6	9.1	13.7

