
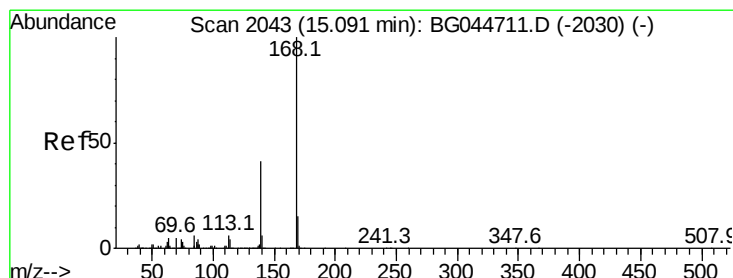
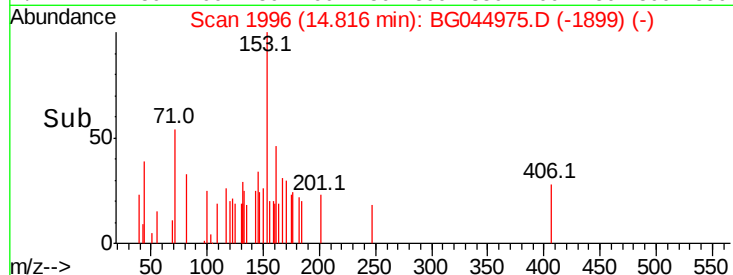
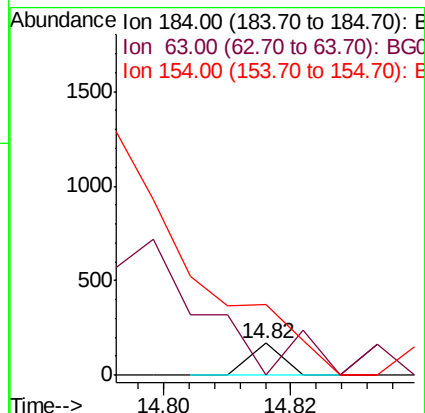


#54
2,4-Dinitrophenol
Concen: 8.346 ng
RT: 14.82 min Scan# 1996
Delta R.T. 0.04 min
Lab File: BG044975.D
Acq: 8 Apr 2020 13:59

Instrument :
BNA_G
ClientSampleId :

Tot Ion:184 Resp: 60
Ion Ratio Lower Upper
184 100
63 0.0 45.5 68.3#
154 220.6 49.1 73.7#

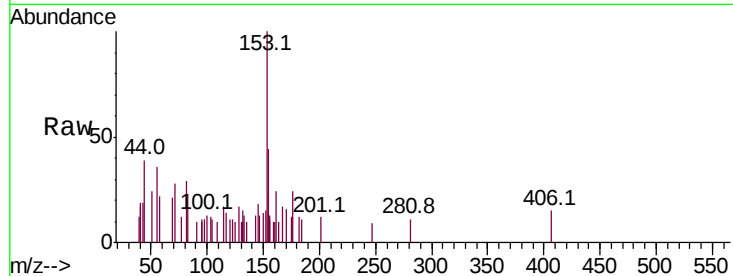

#55
Dibenzofuran
Concen: 4.565 ng
RT: 15.07 min Scan# 2039
Delta R.T. -0.01 min
Lab File: BG044975.D
Acq: 8 Apr 2020 13:59

Tgt Ion:168 Resp: 116127
Ion Ratio Lower Upper
168 100
139 37.1 31.4 47.0
169 18.4 11.1 16.7#

