
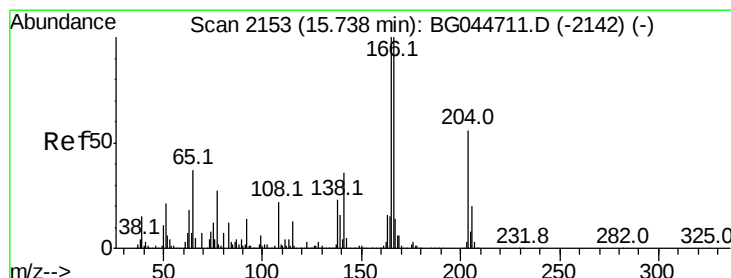
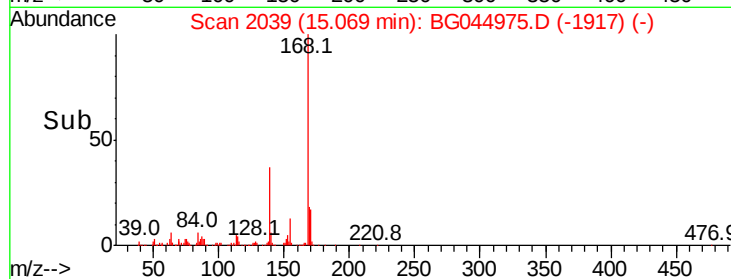
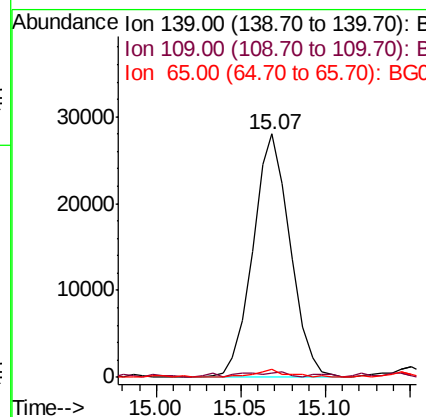


#56
4-Nitrophenol
Concen: 10.847 ng
RT: 15.07 min Scan# 2039
Delta R.T. 0.19 min
Lab File: BG044975.D
Acq: 8 Apr 2020 13:59

Instrument :
BNA_G
ClientSampleId :

Tot Ion:139 Resp: 42796
Ion Ratio Lower Upper
139 100
109 2.0 68.8 108.8#
65 3.5 92.5 132.5#

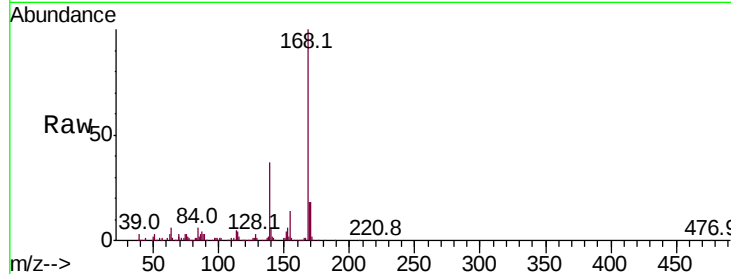

#58
Fluorene
Concen: 4.650 ng
RT: 15.72 min Scan# 2150
Delta R.T. -0.01 min
Lab File: BG044975.D
Acq: 8 Apr 2020 13:59

Tgt Ion:166 Resp: 97302
Ion Ratio Lower Upper
166 100
165 95.1 79.7 119.5
167 14.1 10.6 16.0

