
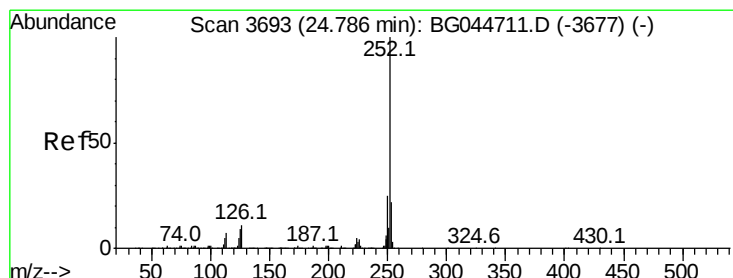
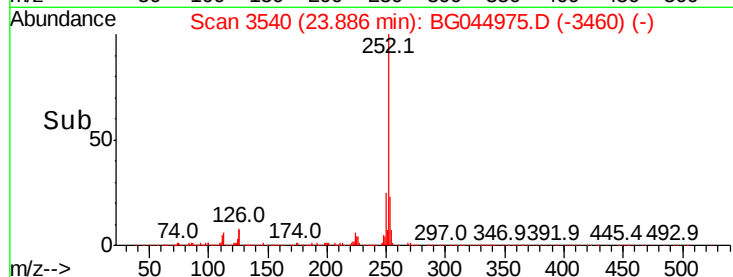
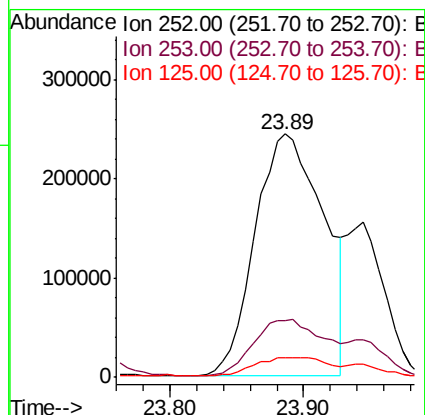


#89
Benzo(k)fluoranthene
Concen: 27.680 ng
RT: 23.89 min Scan# 3540
Delta R.T. -0.06 min
Lab File: BG044975.D
Acq: 8 Apr 2020 13:59

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.3	18.5	27.7
125	8.0	6.2	9.2

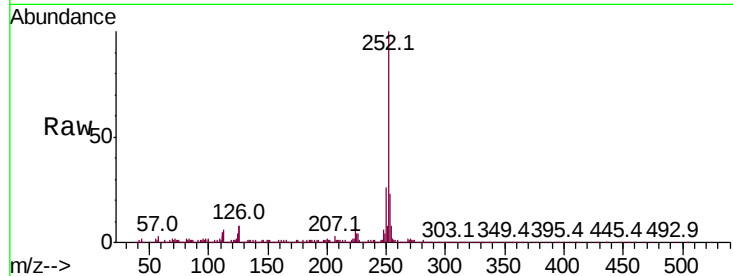

#90
Benzo(a)pyrene
Concen: 19.302 ng
RT: 24.74 min Scan# 3686
Delta R.T. -0.00 min
Lab File: BG044975.D
Acq: 8 Apr 2020 13:59

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.1	19.4	29.0
125	8.0	7.2	10.8

