
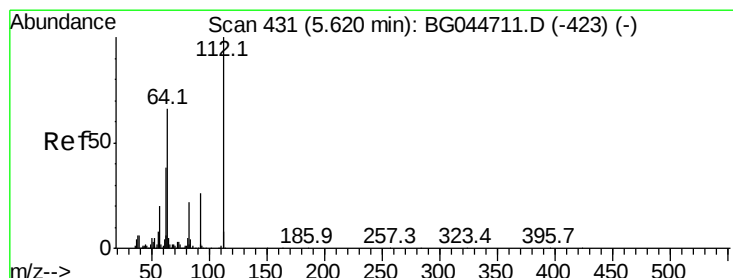
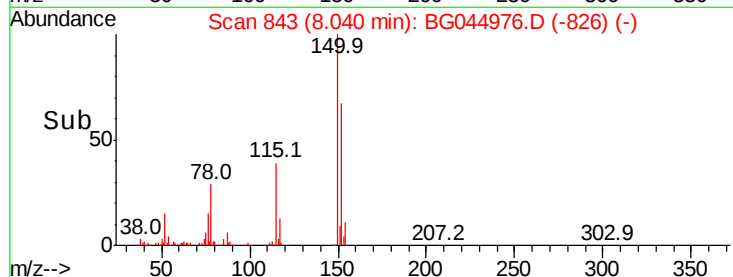
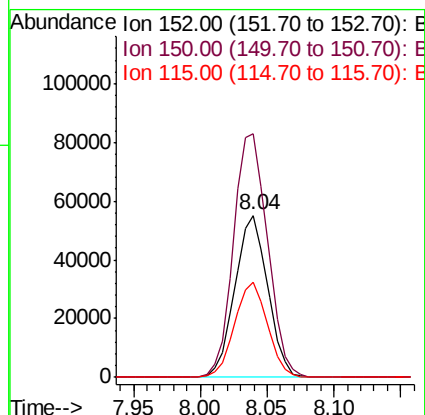


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.04 min Scan# 843
 Delta R.T. -0.00 min
 Lab File: BG044976.D
 Acq: 8 Apr 2020 14:38

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	150.1	128.8	193.2
115	58.3	52.6	79.0

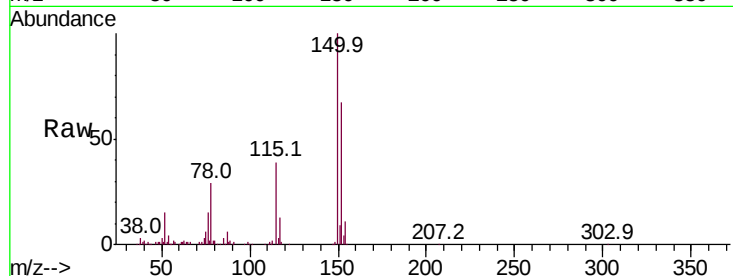

#5

2-Fluorophenol
 Concen: 31.032 ng
 RT: 5.61 min Scan# 429
 Delta R.T. -0.00 min
 Lab File: BG044976.D
 Acq: 8 Apr 2020 14:38

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.9	53.4	80.2
63	32.9	29.4	44.2

