
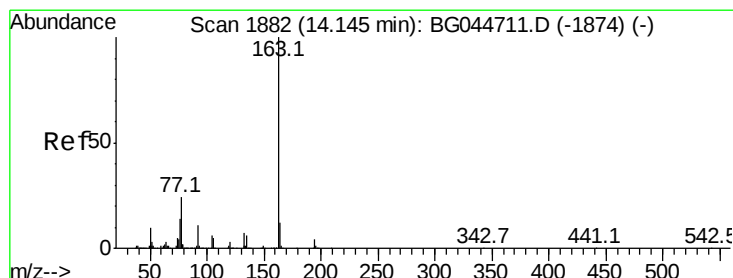
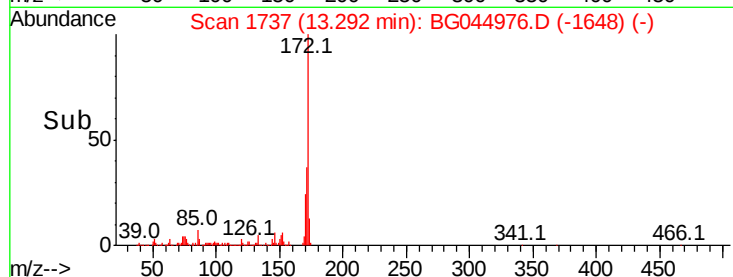
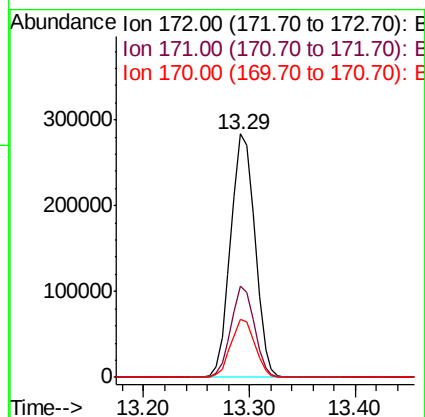


#45
2-Fluorobiphenyl
Concen: 23.563 ng
RT: 13.29 min Scan# 1737
Delta R.T. -0.01 min
Lab File: BG044976.D
Acq: 8 Apr 2020 14:38

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
172	100		
171	37.3	28.7	43.1
170	23.9	19.0	28.6

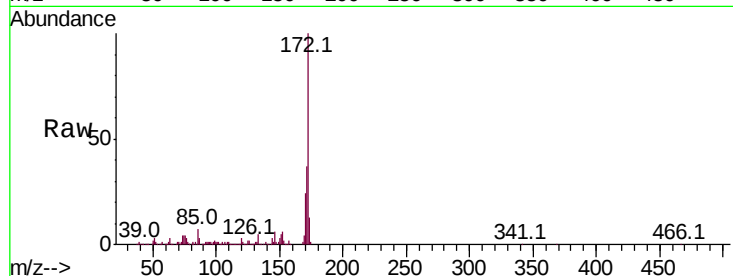

#50
Dimethylphthalate
Concen: 2.153 ng
RT: 14.12 min Scan# 1878
Delta R.T. -0.01 min
Lab File: BG044976.D
Acq: 8 Apr 2020 14:38

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.7	5.5
164	10.5	9.1	13.7

