

#72

Anthracene

Concen: 2.073 ng

RT: 17.54 min Scan# 2461

Delta R.T. -0.01 min

Lab File: BG044976.D

Acq: 8 Apr 2020 14:38

Instrument :

BNA_G

ClientSampled :


Tot Ion:178 Resp: 64083

Ion Ratio Lower Upper

178 100

176 20.4 15.9 23.9




179 17.5 13.2 19.8

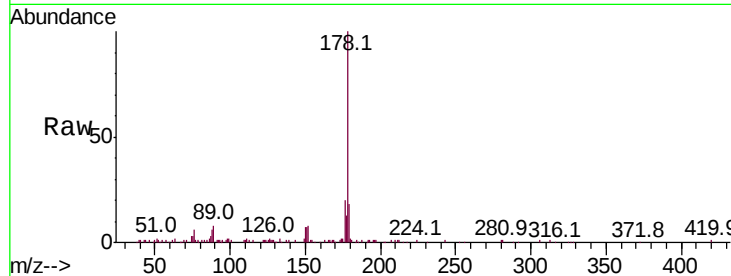

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

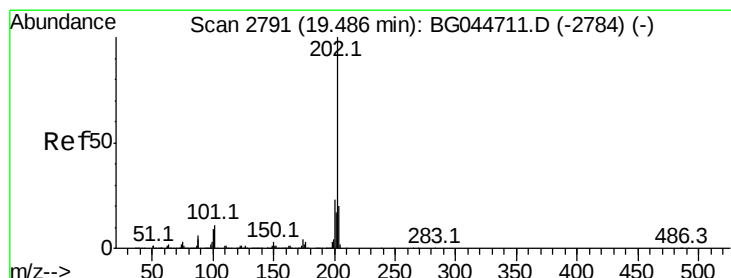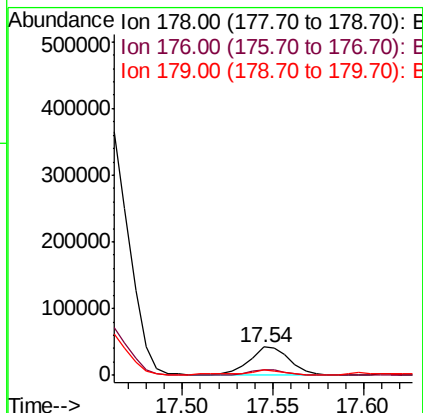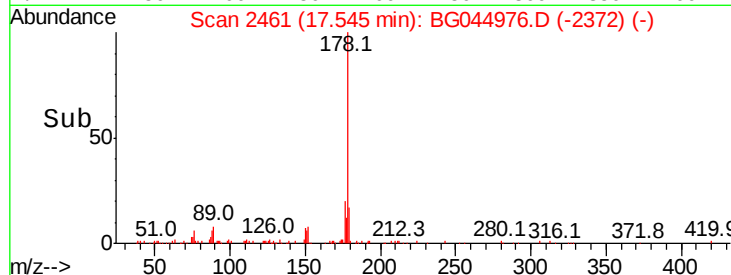

#75

Fluoranthene

Concen: 29.420 ng

RT: 19.47 min Scan# 2788

Delta R.T. -0.00 min

Lab File: BG044976.D

Acq: 8 Apr 2020 14:38


Tgt Ion:202 Resp: 1098028

Ion Ratio Lower Upper

202 100

101 9.2 0.0 29.8

203 19.7 0.0 39.4

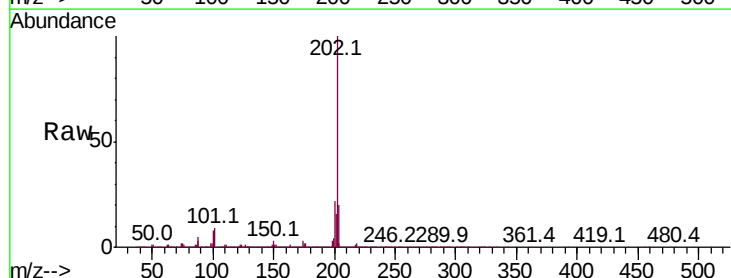

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

