
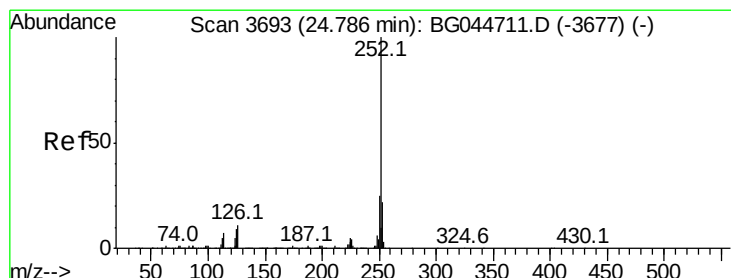
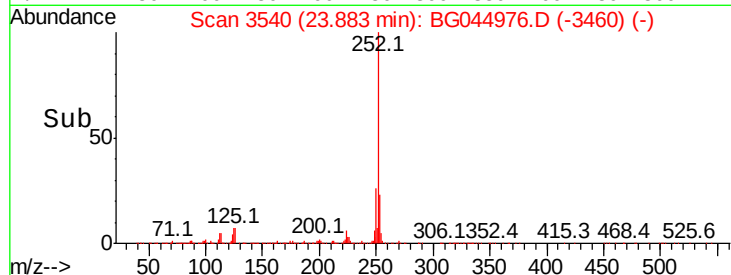
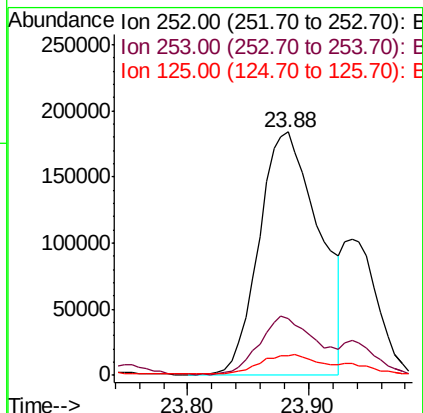


#89
Benzo(k)fluoranthene
Concen: 18.991 ng
RT: 23.88 min Scan# 3540
Delta R.T. -0.06 min
Lab File: BG044976.D
Acq: 8 Apr 2020 14:38

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.4	18.5	27.7
125	7.9	6.2	9.2

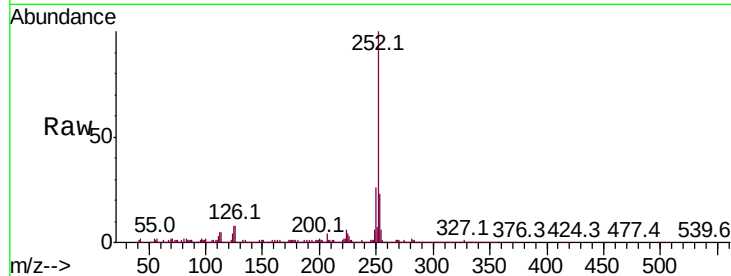

#90
Benzo(a)pyrene
Concen: 13.790 ng
RT: 24.74 min Scan# 3686
Delta R.T. -0.00 min
Lab File: BG044976.D
Acq: 8 Apr 2020 14:38

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.8	19.4	29.0
125	7.4	7.2	10.8

