
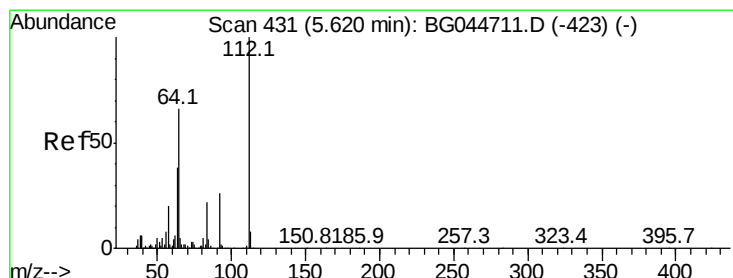
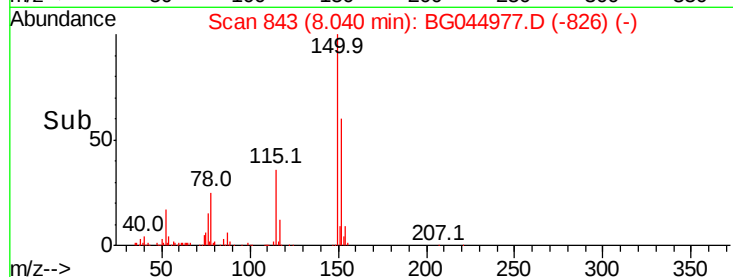
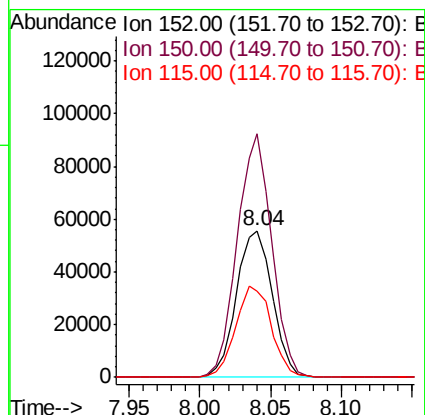


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 843
Delta R.T. -0.00 min
Lab File: BG044977.D
Acq: 8 Apr 2020 15:18

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	166.1	128.8	193.2
115	59.0	52.6	79.0

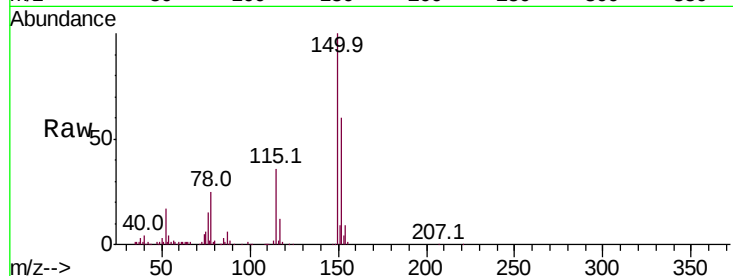

#5

2-Fluorophenol
Concen: 7.436 ng
RT: 5.61 min Scan# 429
Delta R.T. -0.00 min
Lab File: BG044977.D
Acq: 8 Apr 2020 15:18

Tgt Ion	Ratio	Lower	Upper
112	100		
64	51.4	53.4	80.2#
63	28.0	29.4	44.2#

