
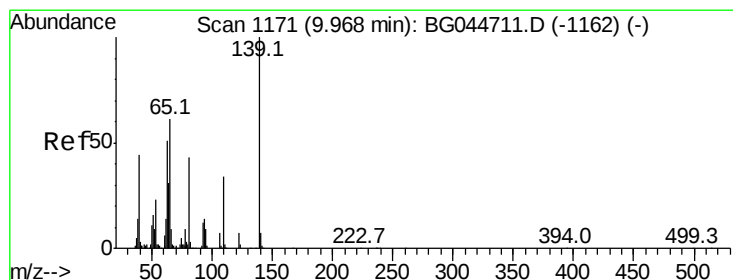
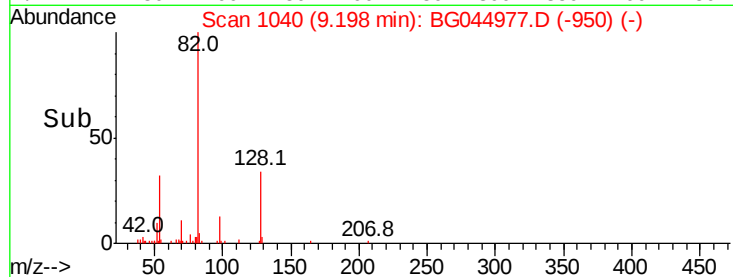
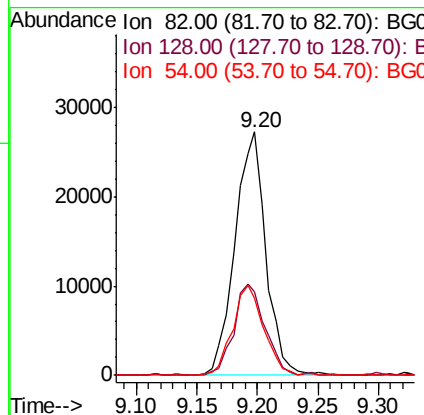


#23
 Nitrobenzene-d5
 Concen: 5.057 ng
 RT: 9.20 min Scan# 1040
 Delta R.T. -0.00 min
 Lab File: BG044977.D
 Acq: 8 Apr 2020 15:18

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	82	Resp	48420
Ion Ratio	100	Lower	Upper
128	34.4	30.6	46.0
54	31.9	37.1	55.7#

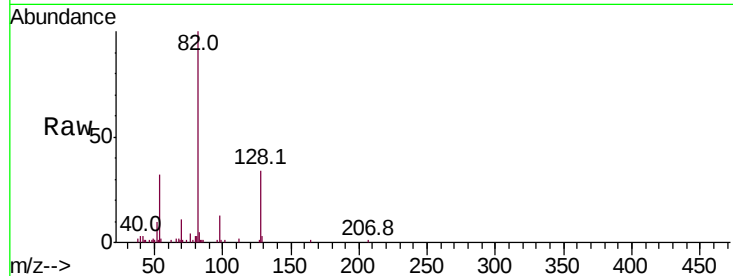

#26
 2-Nitrophenol
 Concen: 5.533 ng
 RT: 10.12 min Scan# 1197
 Delta R.T. 0.16 min
 Lab File: BG044977.D
 Acq: 8 Apr 2020 15:18

Tgt Ion	139	Resp	71
Ion Ratio	100	Lower	Upper
109	0.0	30.2	45.4#
65	0.0	46.3	69.5#

