
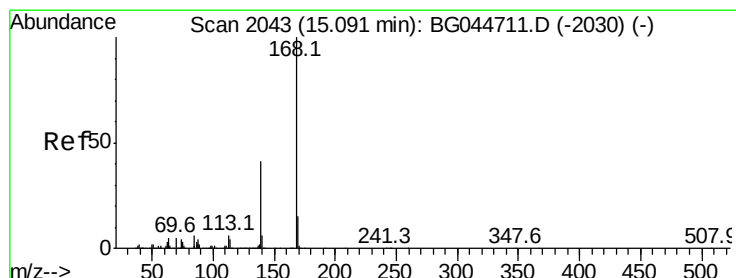
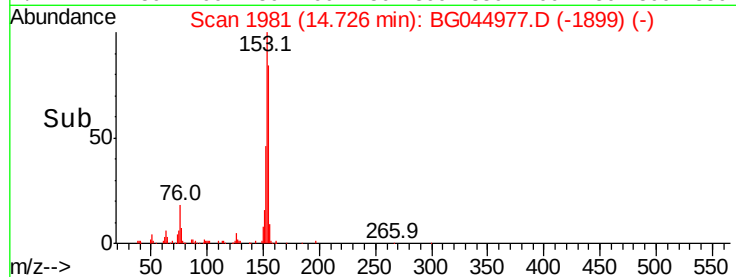
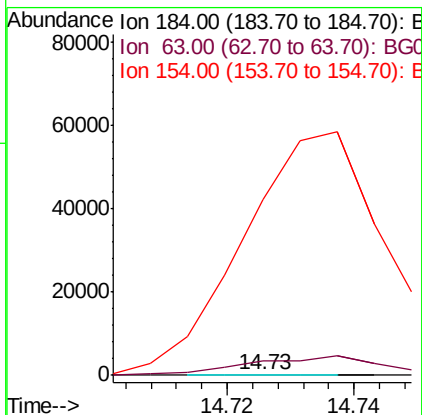


#54
 2,4-Dinitrophenol
 Concen: 8.344 ng
 RT: 14.73 min Scan# 1981
 Delta R.T. -0.05 min
 Lab File: BG044977.D
 Acq: 8 Apr 2020 15:18

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:184 Resp: 59
 Ion Ratio Lower Upper
 184 100
 63 2045.8 45.5 68.3#
 154 25363.9 49.1 73.7#

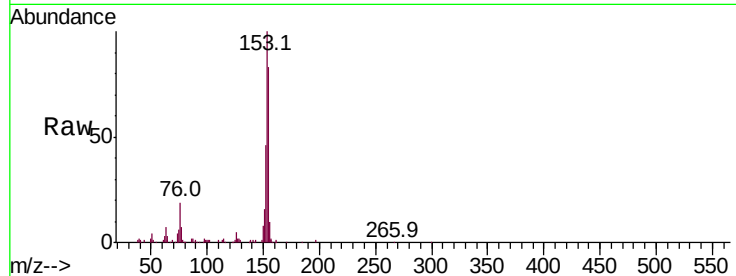

#55
 Dibenzofuran
 Concen: 5.672 ng
 RT: 15.07 min Scan# 2039
 Delta R.T. -0.01 min
 Lab File: BG044977.D
 Acq: 8 Apr 2020 15:18

Tgt Ion:168 Resp: 149079
 Ion Ratio Lower Upper
 168 100
 139 40.1 31.4 47.0
 169 14.1 11.1 16.7

