
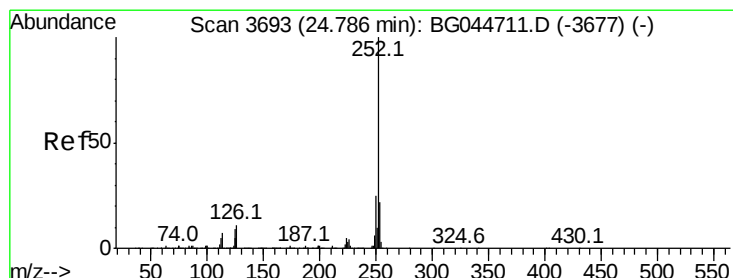
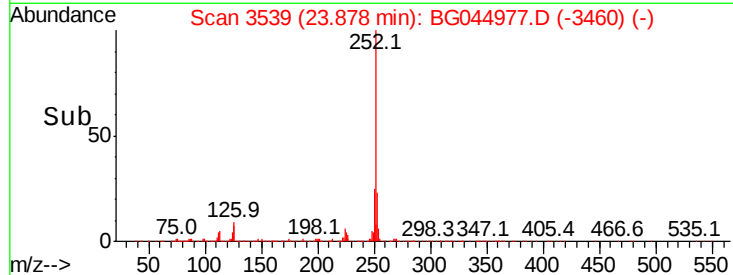
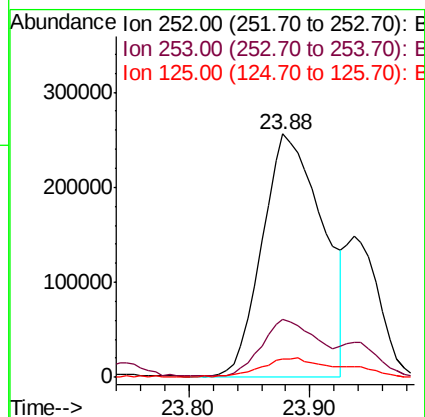


#89
Benzo(k)fluoranthene
Concen: 25.310 ng
RT: 23.88 min Scan# 3539
Delta R.T. -0.07 min
Lab File: BG044977.D
Acq: 8 Apr 2020 15:18

Instrument :
BNA_G
ClientSampleId :

Tot Ion:252 Resp: 883285
Ion Ratio Lower Upper
252 100
253 23.6 18.5 27.7
125 7.5 6.2 9.2

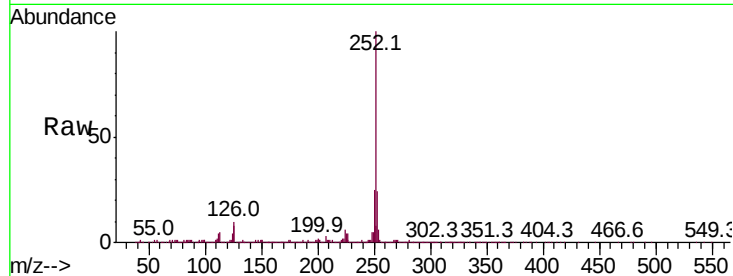

#90
Benzo(a)pyrene
Concen: 18.562 ng
RT: 24.74 min Scan# 3686
Delta R.T. -0.00 min
Lab File: BG044977.D
Acq: 8 Apr 2020 15:18

Tgt Ion:252 Resp: 640502
Ion Ratio Lower Upper
252 100
253 23.8 19.4 29.0
125 7.9 7.2 10.8

