

#91

Dibenzo(a,h)anthracene

Concen: 3.195 ng

RT: 28.56 min Scan# 4336

Delta R.T. -0.04 min

Lab File: BG044977.D

Acq: 8 Apr 2020 15:18


Instrument :

BNA_G

ClientSampleId :

Tot Ion:278 Resp: 108763

Ion	Ratio	Lower	Upper
278	100		
139	14.0	10.2	15.2
279	32.2	18.9	28.3



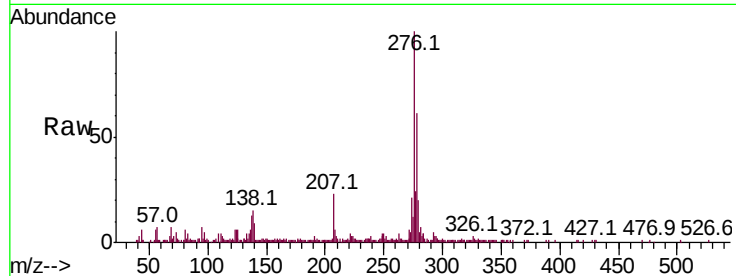


Abundance

Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

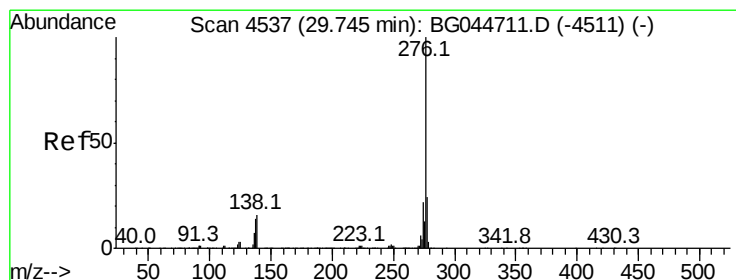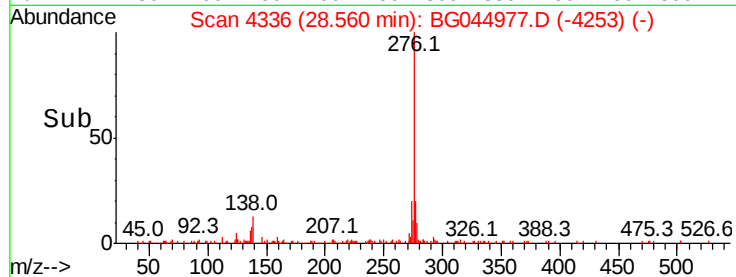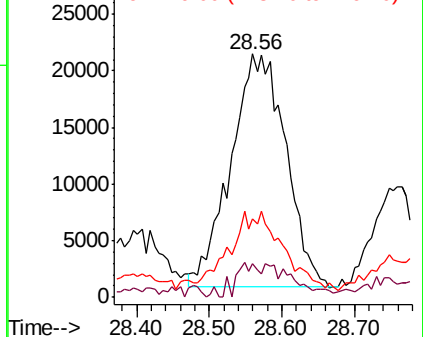

#92

Benzo(g,h,i)perylene

Concen: 8.861 ng

RT: 29.66 min Scan# 4524


Delta R.T. -0.01 min

Lab File: BG044977.D

Acq: 8 Apr 2020 15:18

Tgt Ion:276 Resp: 304767

Ion	Ratio	Lower	Upper
276	100		
277	23.7	20.1	30.1
138	12.3	13.0	19.6

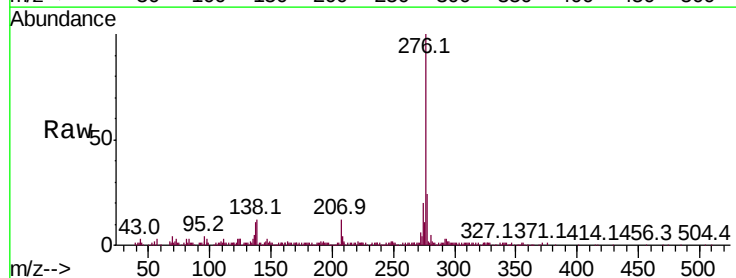

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

