


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG040820\
 Data File : BG044971.D
 Acq On : 8 Apr 2020 10:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG031020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 08 13:01:06 2020

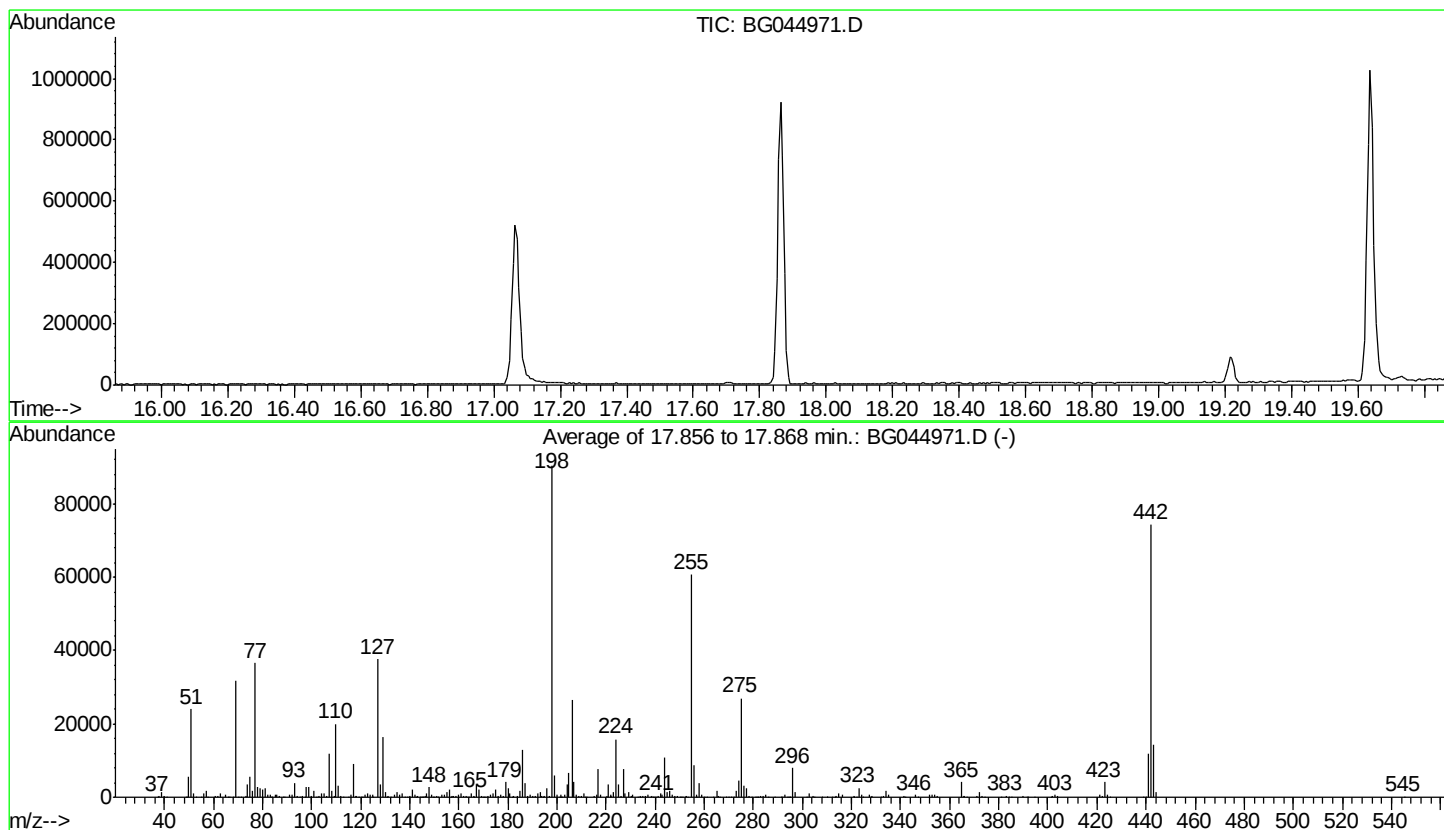

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	23952	PASS
68	69	0.00	2	0.6	183	PASS
69	198	0.00	100	35.3	31922	PASS
70	69	0.00	2	0.6	176	PASS
127	198	10	80	41.6	37642	PASS
197	198	0.00	2	0.3	252	PASS
198	198	100	100	100.0	90378	PASS
199	198	5	9	6.4	5791	PASS
275	198	10	60	29.9	27029	PASS
365	198	1	100	4.5	4092	PASS
441	198	0.01	100	13.0	11763	PASS
442	198	50	100	82.2	74280	PASS
443	442	15	24	19.2	14250	PASS