
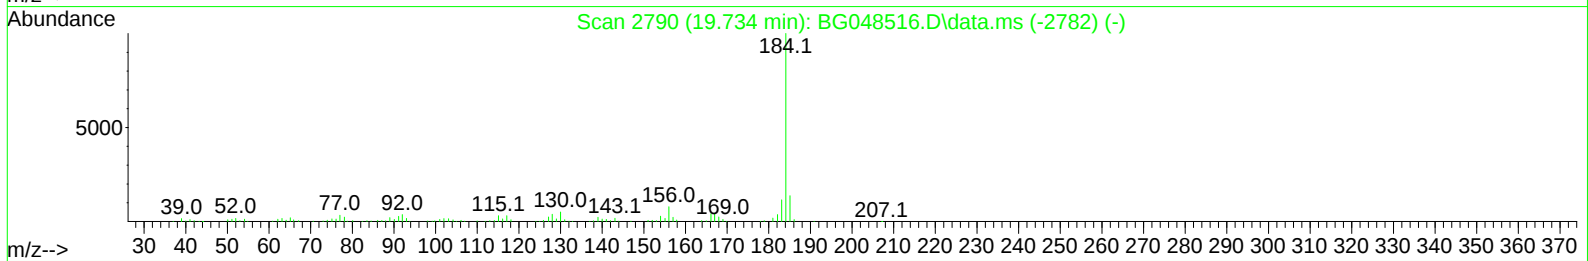
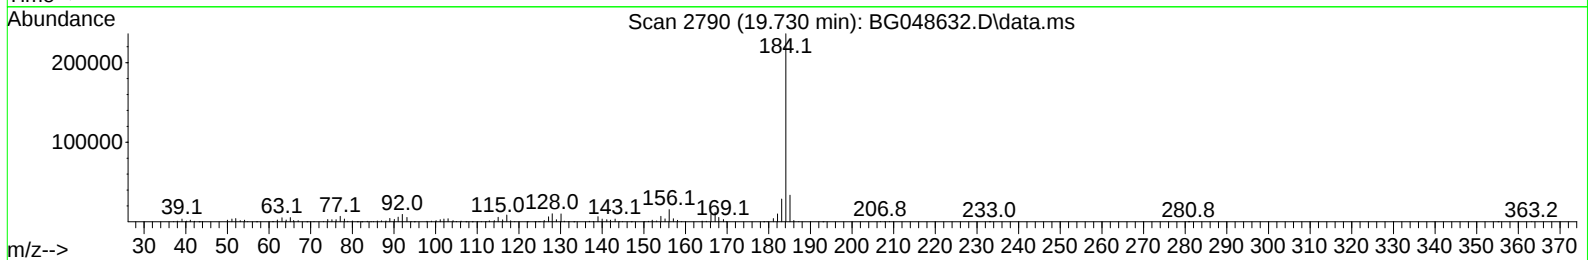


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040821\
 Data File : BG048632.D
 Acq On : 8 Apr 2021 9:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 11:15:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 07 10:06:00 2021
 Response via : Initial Calibration

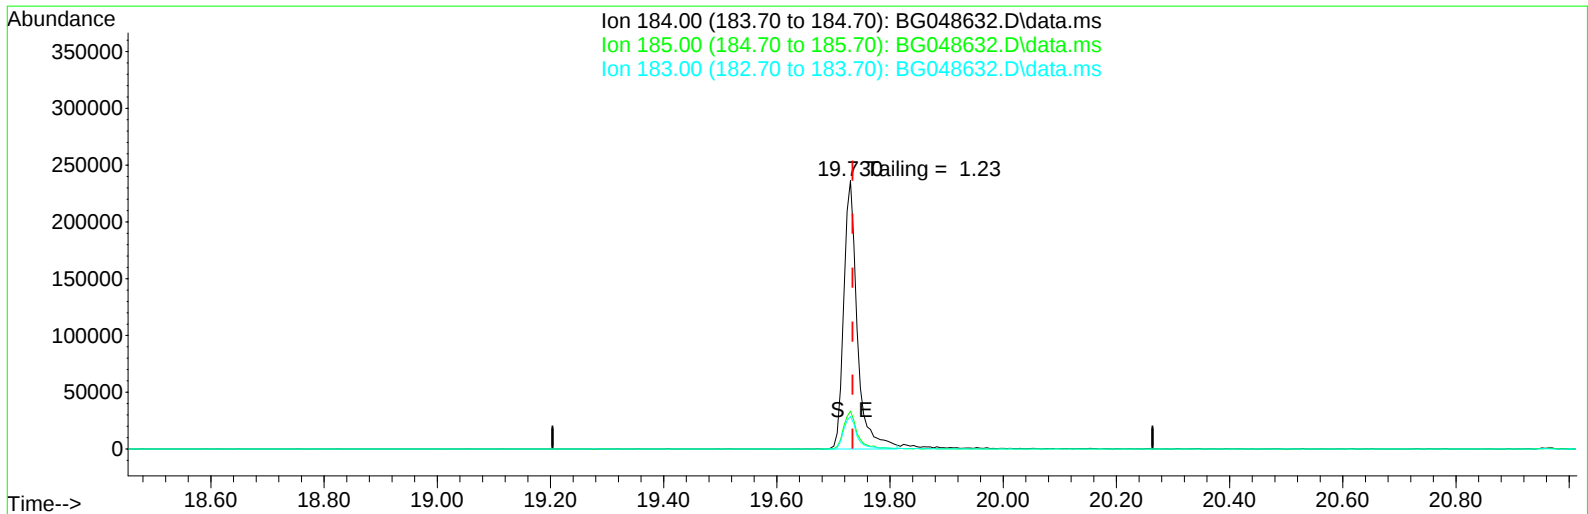

TIC: BG048632.D\data.ms

(77) Benzidine


19.730min (-0.004) 161346.95 ng

response 393386

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.15
183.00	11.50	12.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040821\
Data File : BG048632.D
Acq On : 8 Apr 2021 9:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 11:15:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

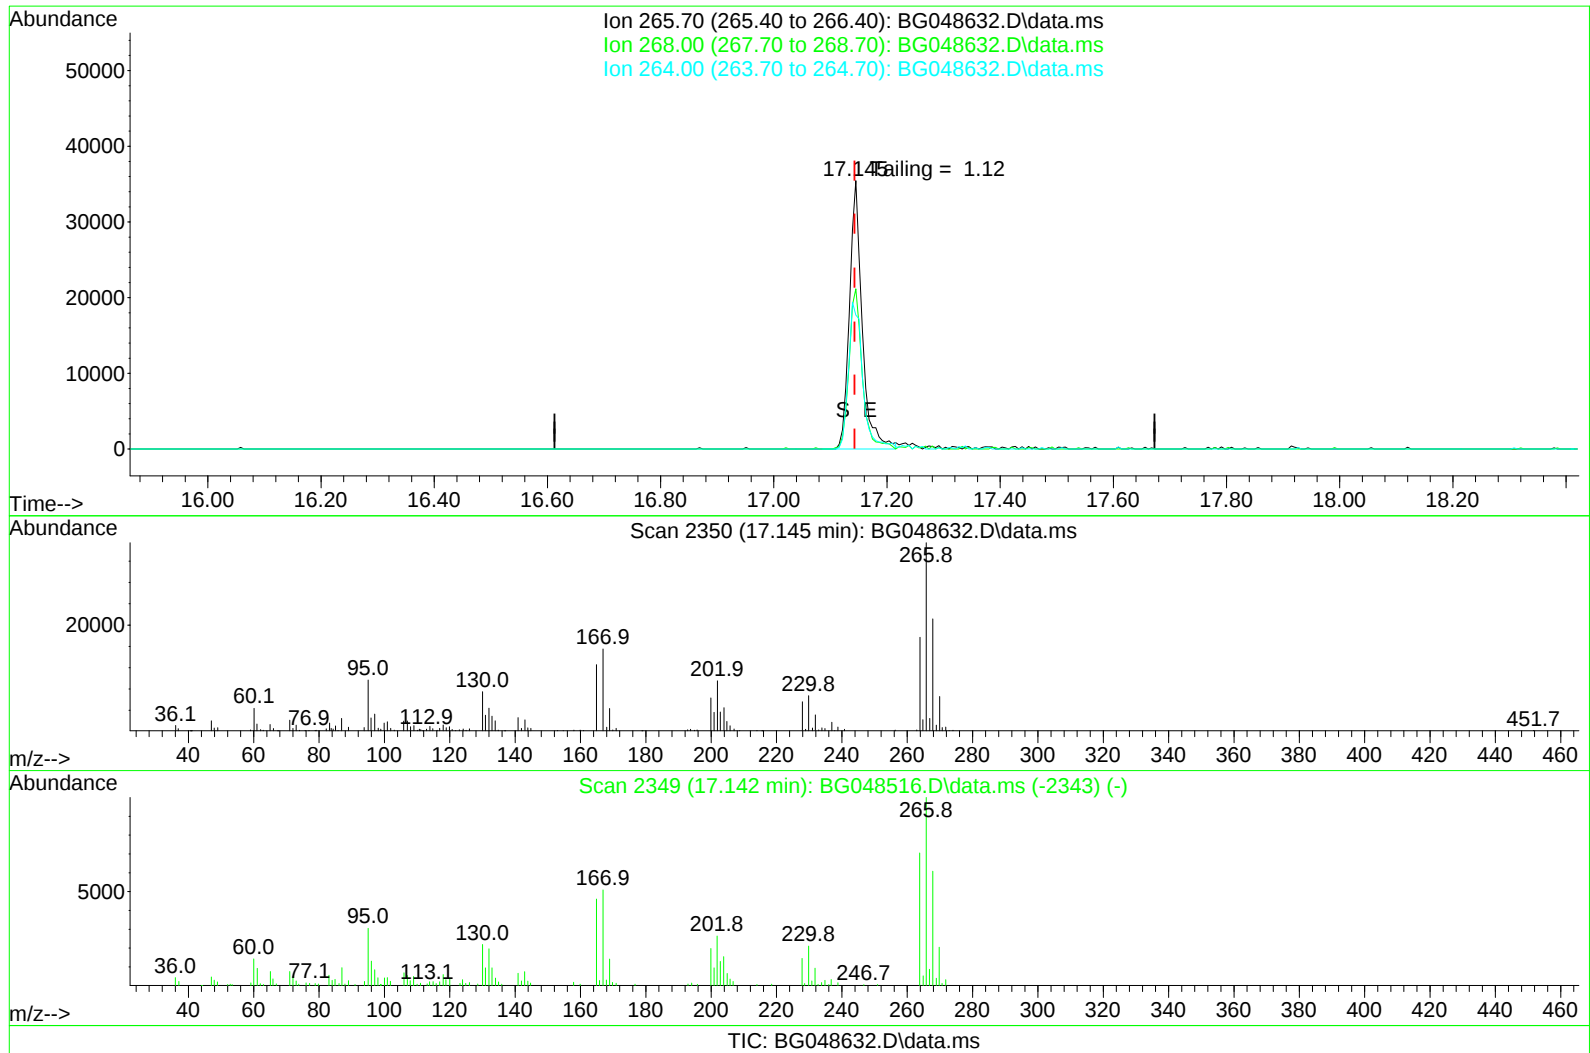**(70) Pentachlorophenol (C)**

17.145min (+ 0.002) 85852.86 ng

response 56206

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	59.67
264.00	70.50	49.90#
0.00	0.00	0.00