

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040821\
 Data File : BG048639.D
 Acq On : 8 Apr 2021 14:54
 Operator : CG/JU
 Sample : M1961-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TR1-A-D-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.634	384	391	401	rBV	298278	475777	32.14%	7.595%
2	7.238	657	664	674	rBV	298027	508754	34.37%	8.122%
3	8.090	802	809	815	rBV	86244	141338	9.55%	2.256%
4	9.254	1001	1007	1014	rBV	176154	319716	21.60%	5.104%
5	10.917	1282	1290	1298	rBV	106526	184037	12.43%	2.938%
6	13.361	1699	1706	1714	rBV	451857	703931	47.55%	11.238%
7	14.183	1841	1846	1854	rBV	11568	19558	1.32%	0.312%
8	14.741	1933	1941	1951	rBV	154278	256775	17.35%	4.099%
9	16.228	2188	2194	2209	rBV	458207	818453	55.29%	13.066%
10	17.497	2403	2410	2416	rBV	251621	391345	26.44%	6.248%
11	17.609	2425	2429	2435	rVB5	11021	16449	1.11%	0.263%
12	20.106	2848	2854	2864	rBV	1091248	1480367	100.00%	23.633%
13	21.410	3071	3076	3086	rBV6	54356	132687	8.96%	2.118%
14	21.792	3134	3141	3150	rBV	237587	430223	29.06%	6.868%
15	25.129	3700	3709	3721	rBV2	123585	384547	25.98%	6.139%




Sum of corrected areas: 6263957

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040821\
Data File : BG048639.D
Acq On : 8 Apr 2021 14:54
Operator : CG/JU
Sample : M1961-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR1-A-D-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

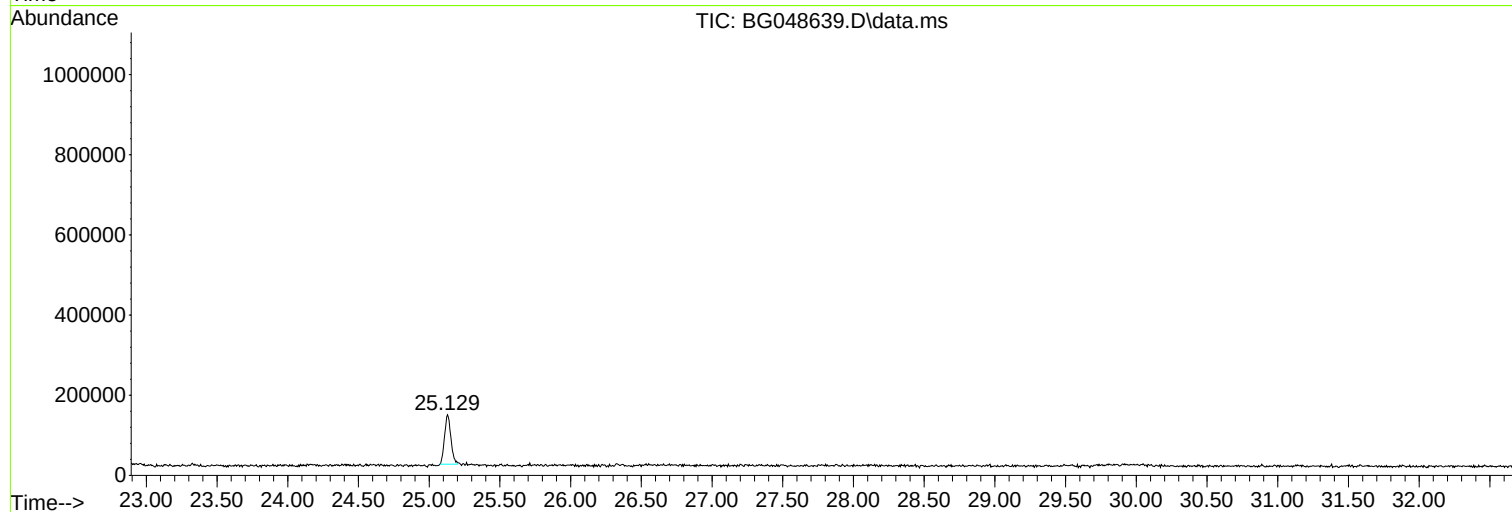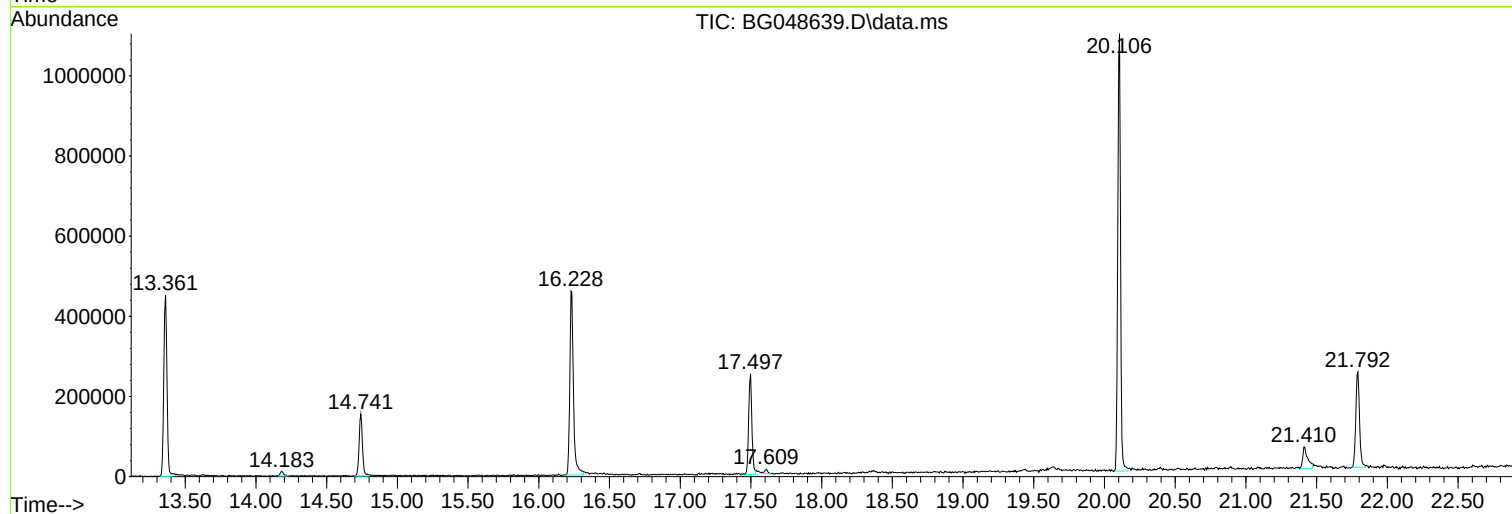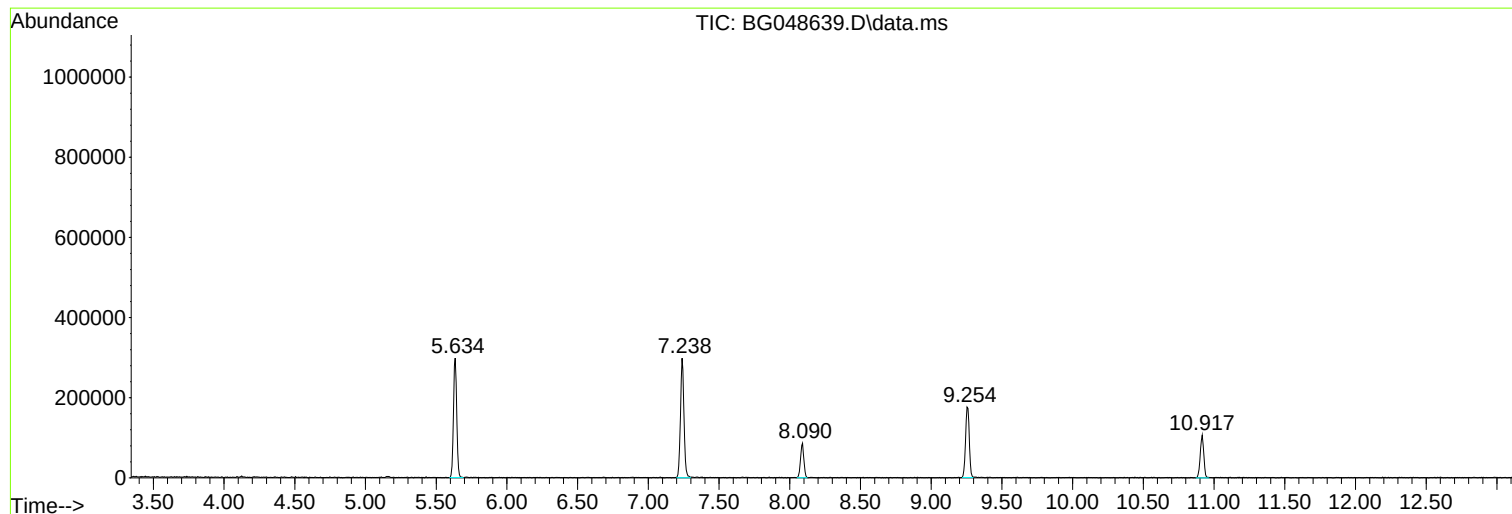

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040821\
Data File : BG048639.D
Acq On : 8 Apr 2021 14:54
Operator : CG/JU
Sample : M1961-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR1-A-D-COMP










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trifluoroacetoxy hexadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.410	6.17 ng	132687	Chrysene-d12	21.786

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	90
2			3-Eicosene, (E)-	280	C20H40	074685-33-9	90
3			Bromoacetic acid, octadecyl ester	390	C20H39BrO2	018992-03-5	87
4			9-Eicosene, (E)-	280	C20H40	074685-29-3	83
5			3-Octadecene, (E)-	252	C18H36	007206-19-1	74

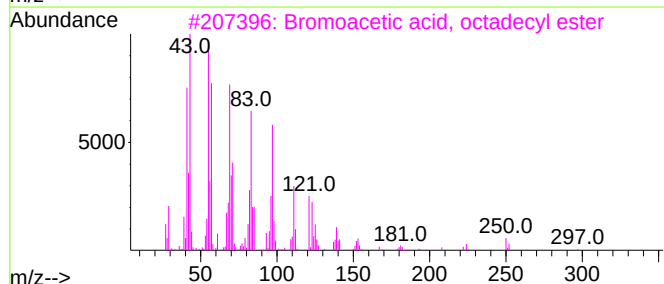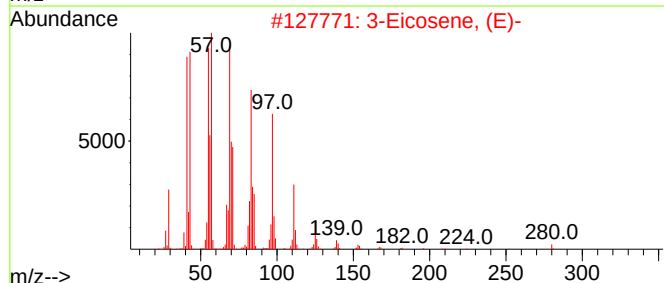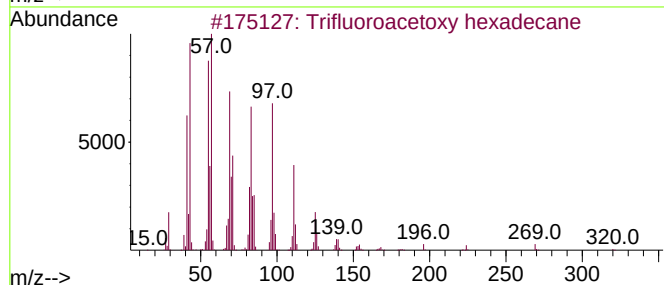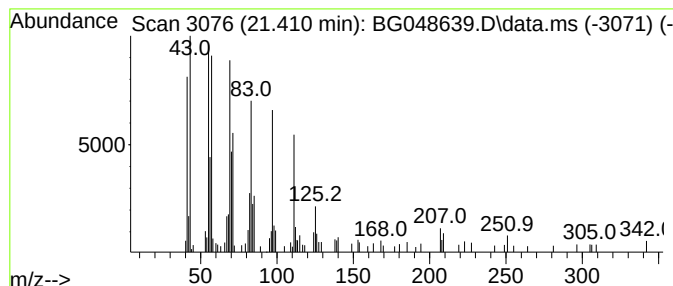

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040821\
Data File : BG048639.D
Acq On : 8 Apr 2021 14:54
Operator : CG/JU
Sample : M1961-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TR1-A-D-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trifluoroacetox...	21.410	6.2	ng	132687	5	21.786	430223	20.0