
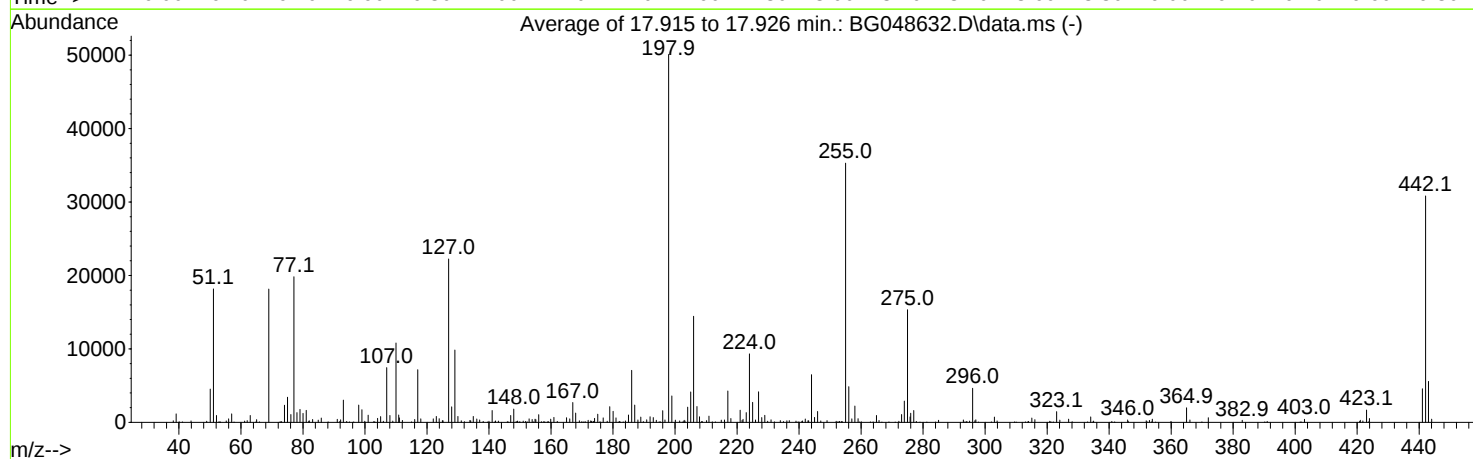


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040821\
 Data File : BG048632.D
 Acq On : 8 Apr 2021 9:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 07 10:06:00 2021

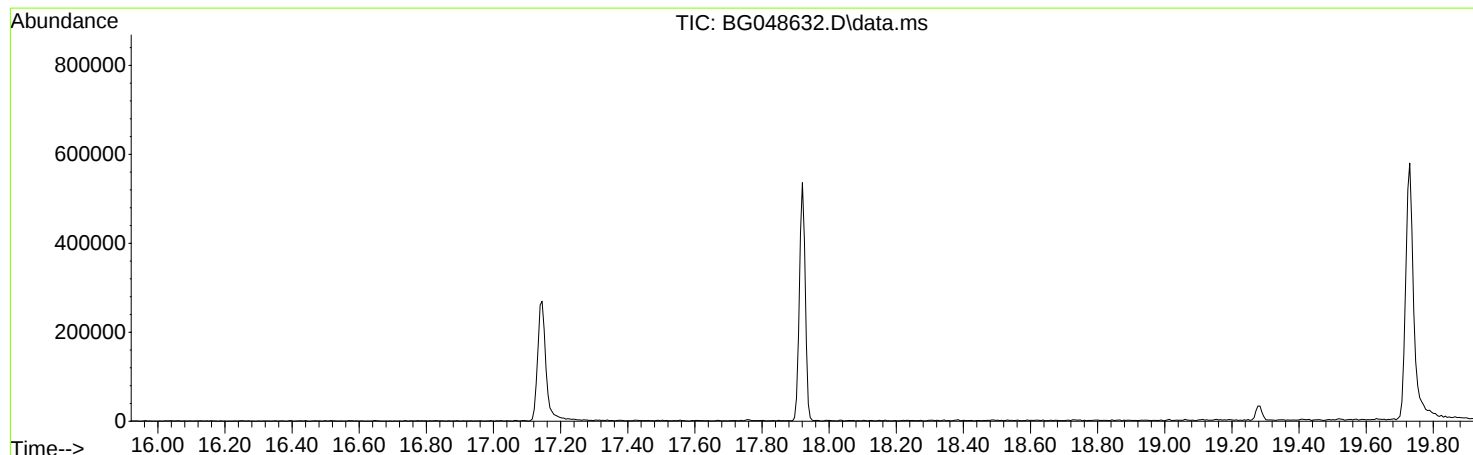

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	18175	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.2	18140	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.4	22243	PASS
197	198	0.00	2	0.6	321	PASS
198	198	100	100	100.0	50083	PASS
199	198	5	9	7.2	3594	PASS
275	198	10	60	30.6	15337	PASS
365	198	1	100	4.0	1981	PASS
441	198	0.01	100	9.1	4581	PASS
442	198	50	100	61.6	30835	PASS
443	442	15	24	18.1	5587	PASS

Instrument :
BNA_G
ClientSampleId :
DFTPP


DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/9/2021	BNA_G	<u>BG048632.D</u>
Compound Name	Response	Retention Time
DDT	210215	20.96
DDD	3021	20.51
DDE	422	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3443	213658	1.61

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040821\
Data File : BG048632.D
Acq On : 8 Apr 2021 9:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 08 11:15:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

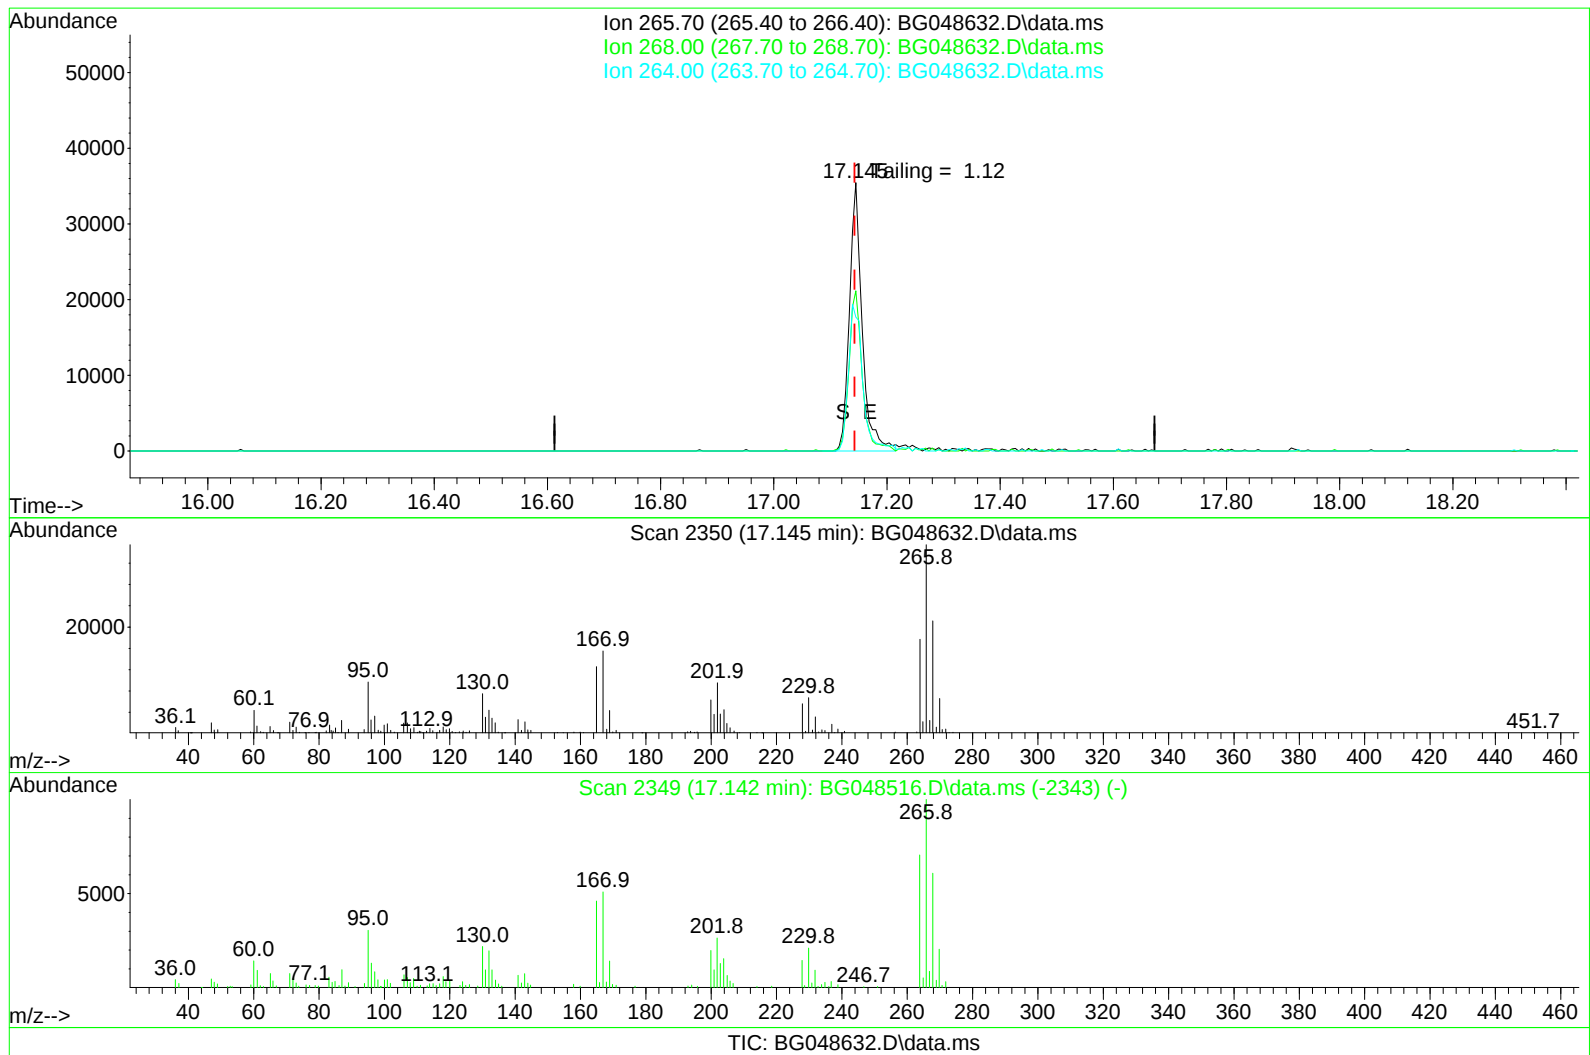

(70) Pentachlorophenol (C)

17.145min (+ 0.002) 85852.86 ng




response 56206

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	59.67
264.00	70.50	49.90#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040821\
 Data File : BG048632.D
 Acq On : 8 Apr 2021 9:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 08 11:15:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 07 10:06:00 2021
 Response via : Initial Calibration

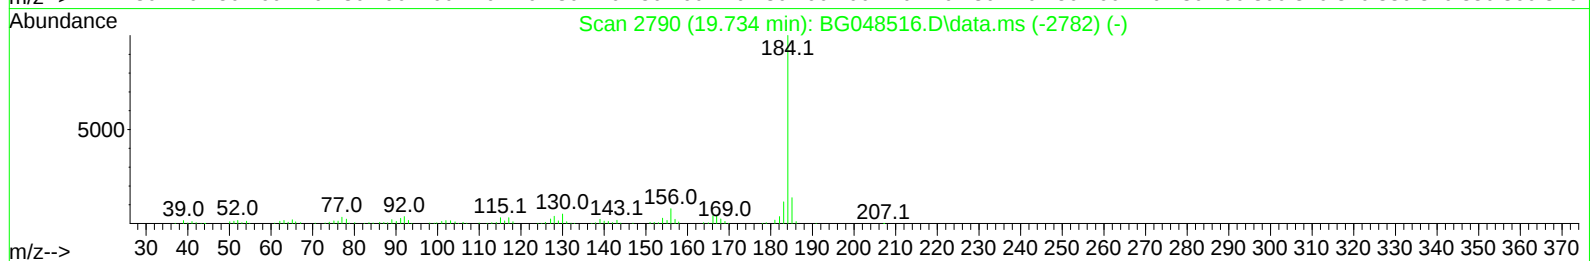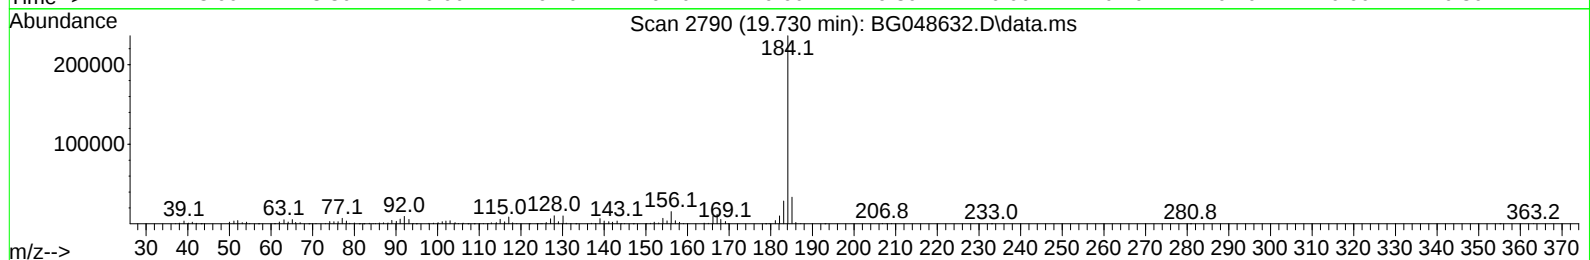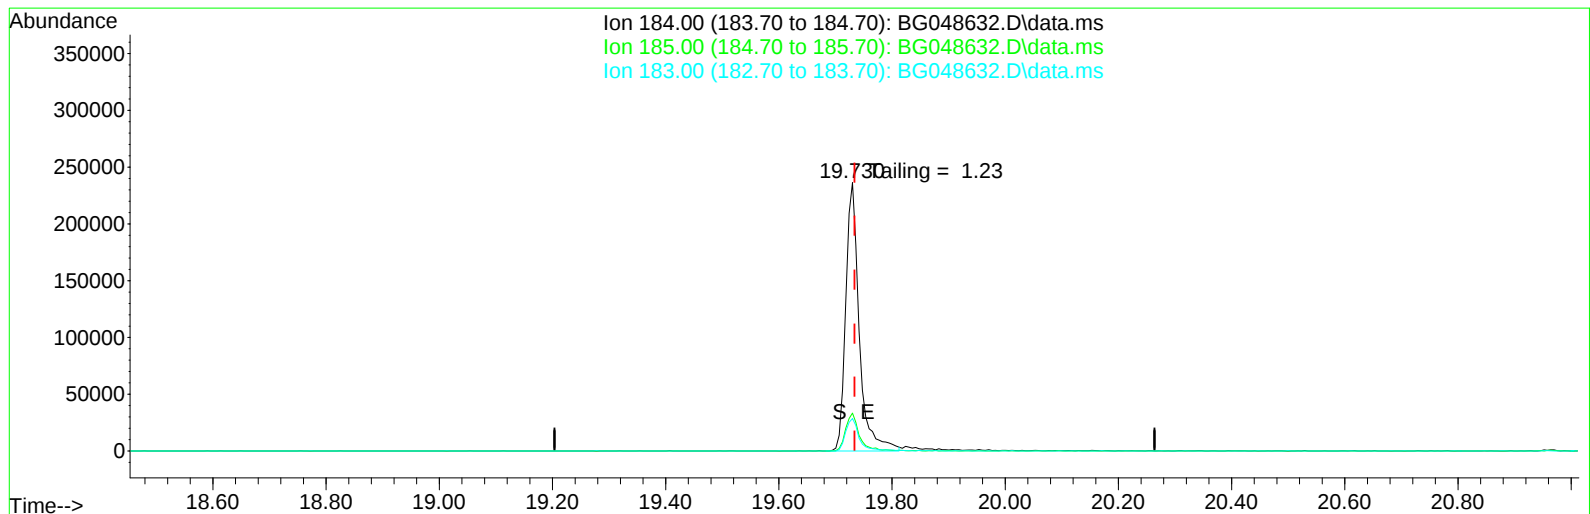

TIC: BG048632.D\data.ms

(77) Benzidine

19.730min (-0.004) 161346.95 ng

response 393386

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.15
183.00	11.50	12.14
0.00	0.00	0.00