


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG041019\
 Data File : BG040430.D
 Acq On : 11 Apr 2019 2:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

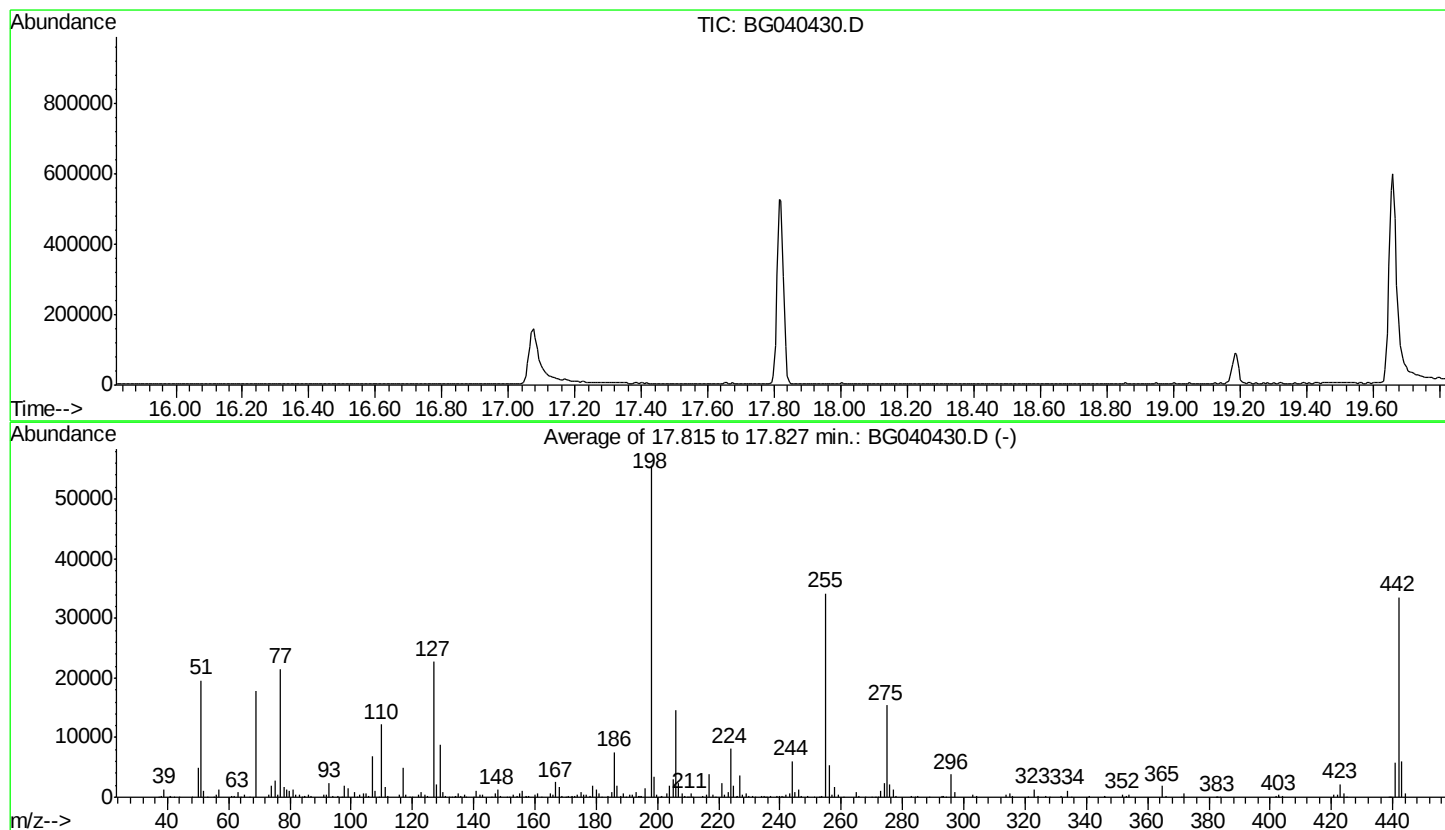

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	19616	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.1	17837	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.8	22674	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55613	PASS
199	198	5	9	6.4	3543	PASS
275	198	10	60	27.7	15424	PASS
365	198	1	100	3.4	1914	PASS
441	198	0.01	100	10.4	5766	PASS
442	198	50	100	60.3	33541	PASS
443	442	15	24	18.0	6031	PASS