

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041119\
 Data File : BG040442.D
 Acq On : 11 Apr 2019 15:28
 Operator : JU/SJ
 Sample : K2360-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FK-BPM-01-E2-E2A-F2-F2A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.602	420	428	445	rBV	739151	1230495	44.23%	7.472%
2	7.201	692	700	721	rBV	759902	1342962	48.27%	8.155%
3	7.577	756	764	779	rBV	730107	1289110	46.34%	7.828%
4	8.047	837	844	856	rVB	211179	365919	13.15%	2.222%
5	8.364	891	898	909	rBV	535417	953342	34.27%	5.789%
6	9.222	1036	1044	1056	rBV	412709	796920	28.65%	4.839%
7	10.861	1315	1323	1333	rBV	253163	492607	17.71%	2.991%
8	13.293	1730	1737	1750	rBV	1122089	1787034	64.24%	10.851%
9	14.122	1873	1878	1891	rBV	110783	180087	6.47%	1.093%
10	14.674	1965	1972	1984	rBV2	412291	693190	24.92%	4.209%
11	16.167	2219	2226	2247	rBV	761671	1340050	48.17%	8.137%
12	17.424	2433	2440	2451	rBV2	543907	895711	32.20%	5.439%
13	20.021	2876	2882	2897	rBV	2106790	2781954	100.00%	16.892%
14	21.296	3095	3099	3105	rBV7	18595	45279	1.63%	0.275%
15	21.689	3159	3166	3179	rBV	598043	1050092	37.75%	6.376%
16	22.442	3290	3294	3301	rVB3	20670	34185	1.23%	0.208%
17	23.135	3407	3412	3418	rVB3	24032	43210	1.55%	0.262%
18	23.323	3440	3444	3455	rVB5	14775	29430	1.06%	0.179%
19	23.940	3542	3549	3558	rVB3	24714	52591	1.89%	0.319%
20	24.886	3703	3710	3711	rBV4	20099	29927	1.08%	0.182%
21	24.968	3715	3724	3745	rVB2	298232	977523	35.14%	5.936%
22	26.031	3894	3905	3913	rBV8	17039	57332	2.06%	0.348%


Sum of corrected areas: 16468950

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041119\
Data File : BG040442.D
Acq On : 11 Apr 2019 15:28
Operator : JU/SJ
Sample : K2360-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-BPM-01-E2-E2A-F2-F2A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

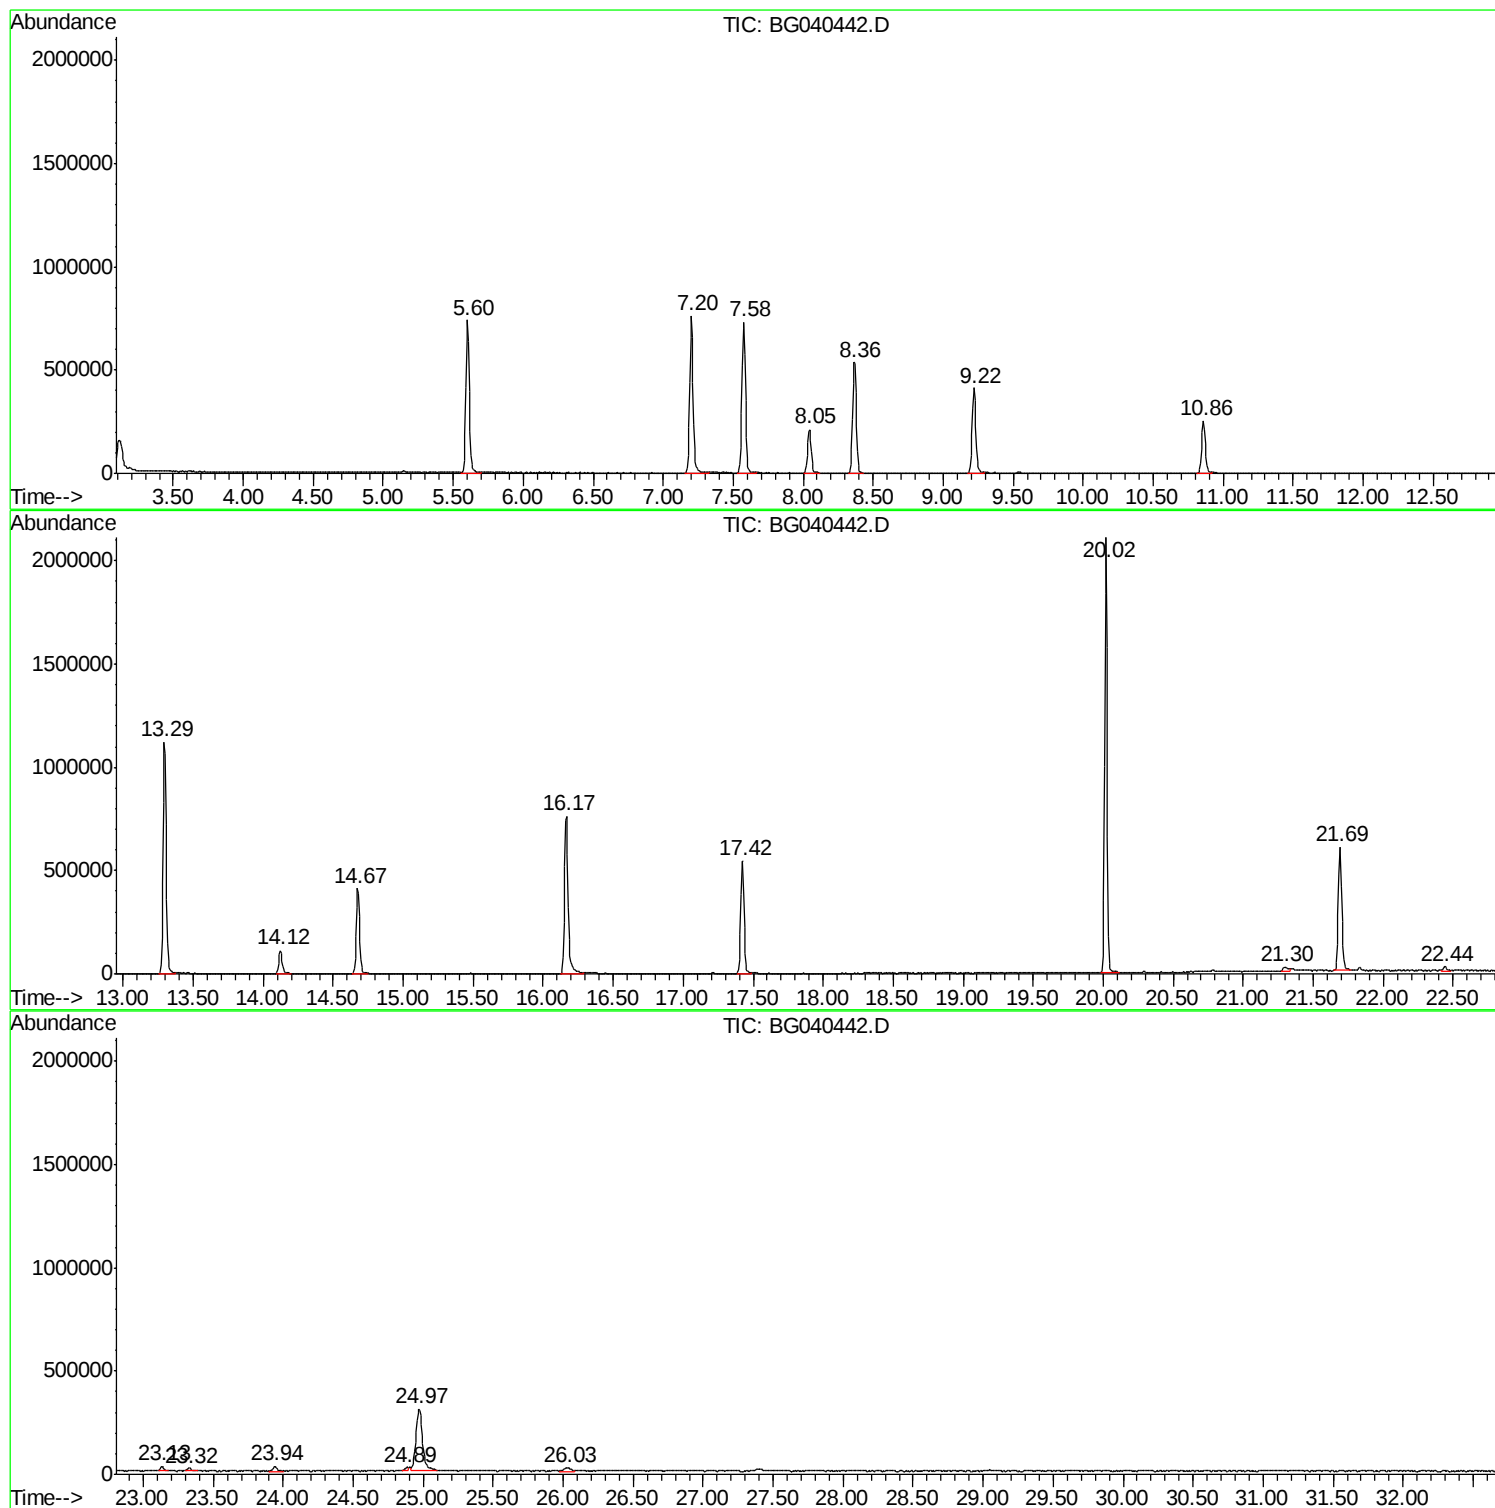

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041119\
Data File : BG040442.D
Acq On : 11 Apr 2019 15:28
Operator : JU/SJ
Sample : K2360-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-BPM-01-E2-E2A-F2-F2A










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	70.46 ng	1289110	1,4-Dichlorobenzene-d4	8.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	22
3		1H-Tetrazaborole, 5-chloro-4,5-d...	132	C2H6BClN4	021960-49-6	16
4		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
5		Amphetaminil	250	C17H18N2	017590-01-1	12

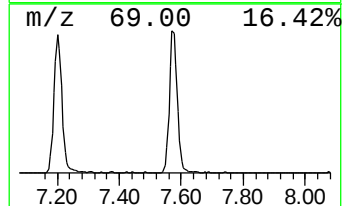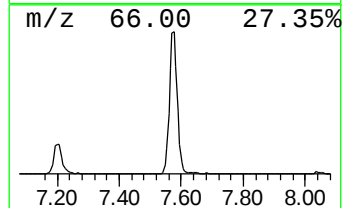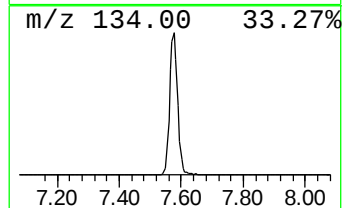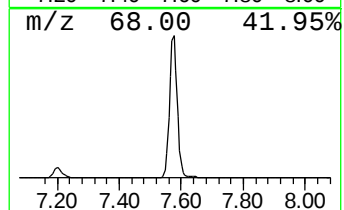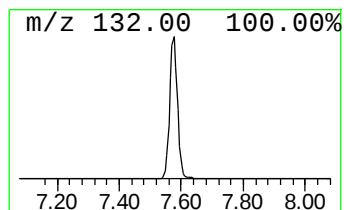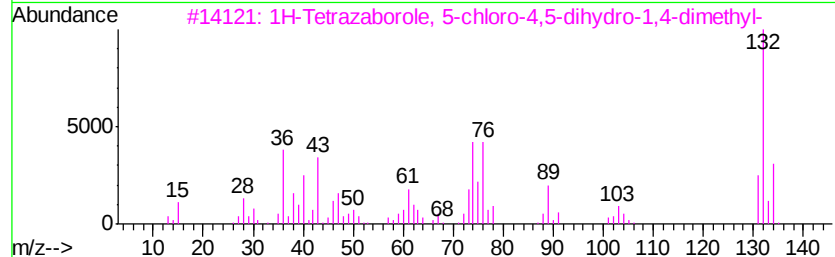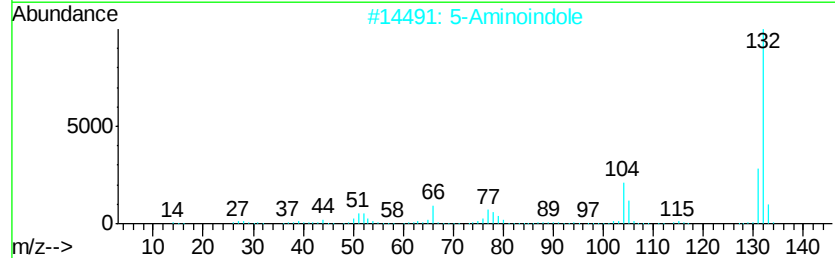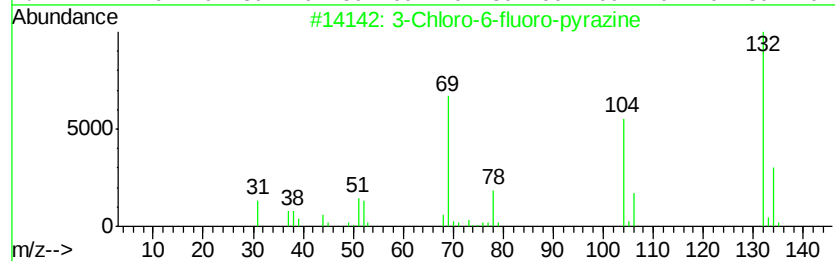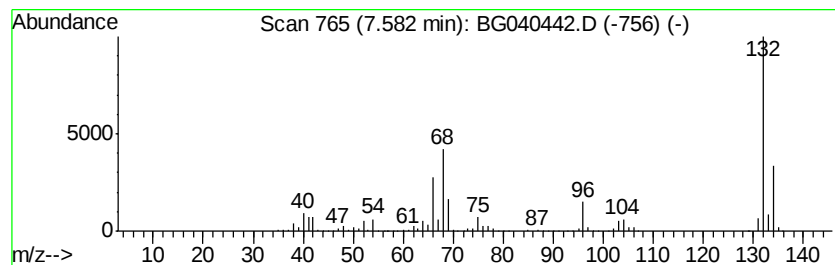

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041119\
Data File : BG040442.D
Acq On : 11 Apr 2019 15:28
Operator : JU/SJ
Sample : K2360-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-BPM-01-E2-E2A-F2-F2A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.58	7.58	70.5	ng	1289110	1	8.05	365919	20.0