


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041119\
 Data File : BG040437.D
 Acq On : 11 Apr 2019 10:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

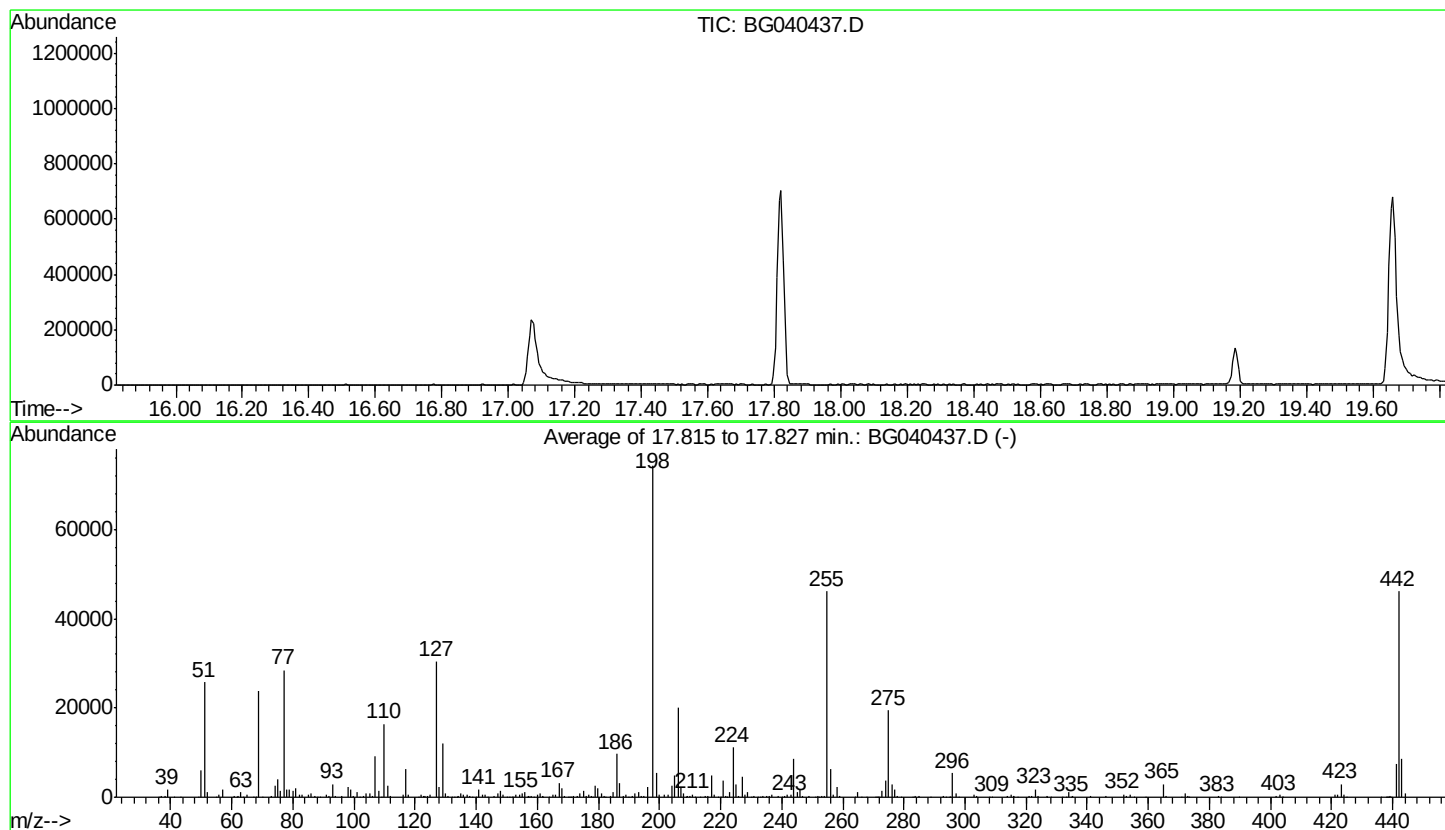

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	25760	PASS
68	69	0.00	2	0.5	120	PASS
69	198	0.00	100	32.0	23777	PASS
70	69	0.00	2	0.2	51	PASS
127	198	10	80	40.8	30336	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74312	PASS
199	198	5	9	7.3	5417	PASS
275	198	10	60	26.2	19442	PASS
365	198	1	100	3.9	2874	PASS
441	198	0.01	100	10.2	7571	PASS
442	198	50	100	62.0	46104	PASS
443	442	15	24	18.8	8662	PASS