
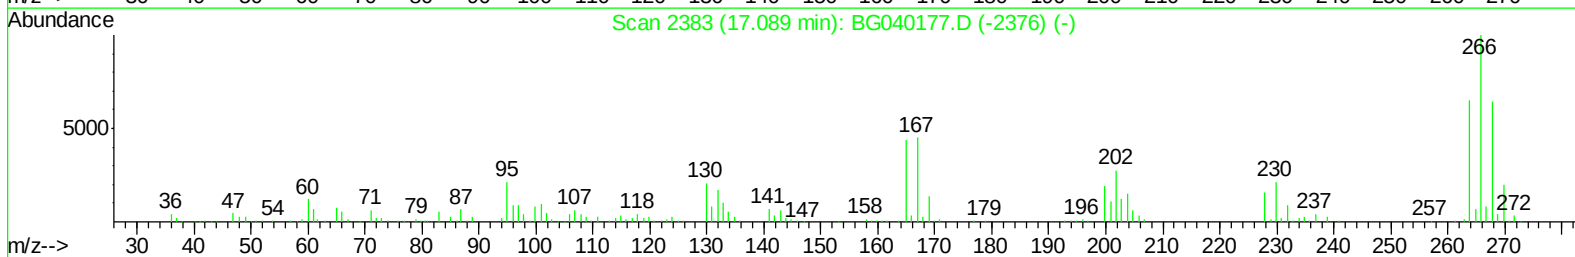
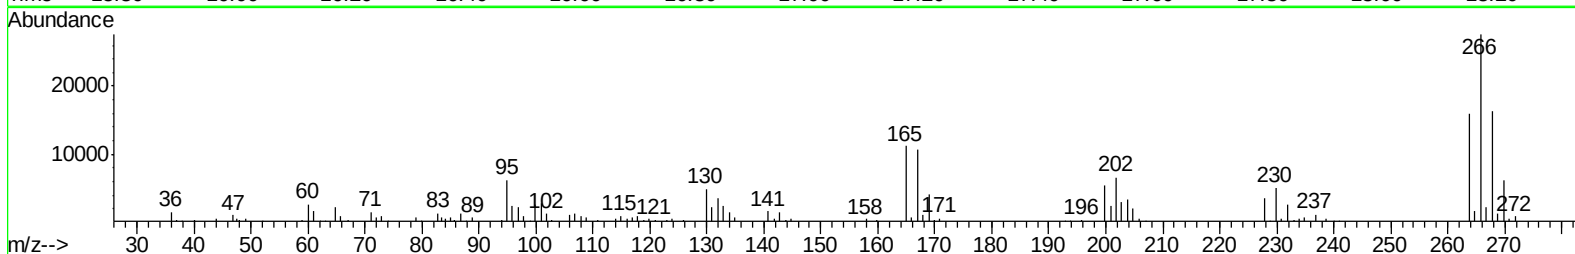


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041219\
Data File : BG040453.D
Acq On : 12 Apr 2019 9:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 05:26:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 00:33:11 2019
Response via : Initial Calibration

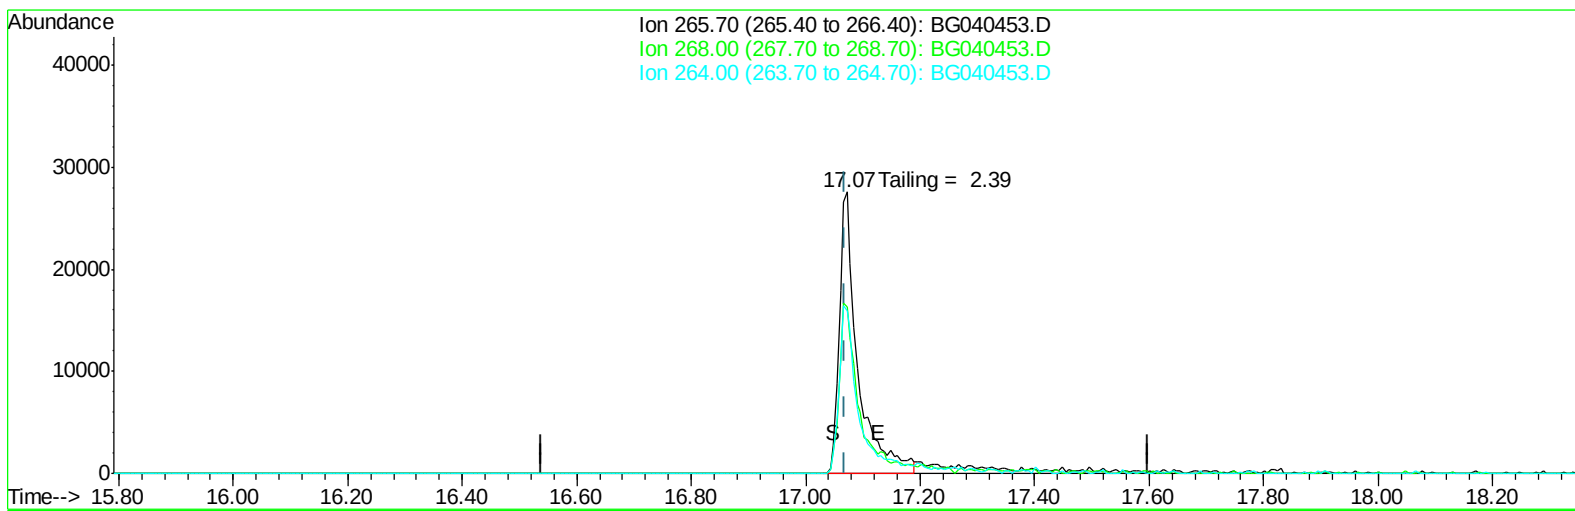

TIC: BG040453.D

(70) Pentachlorophenol (C)




17.072min (+0.003) 171348.64ng

response 61649

Ion	Exp%	Act%
265.70	100	100
268.00	68.70	59.16
264.00	64.80	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041219\
Data File : BG040453.D
Acq On : 12 Apr 2019 9:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 05:26:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 00:33:11 2019
Response via : Initial Calibration

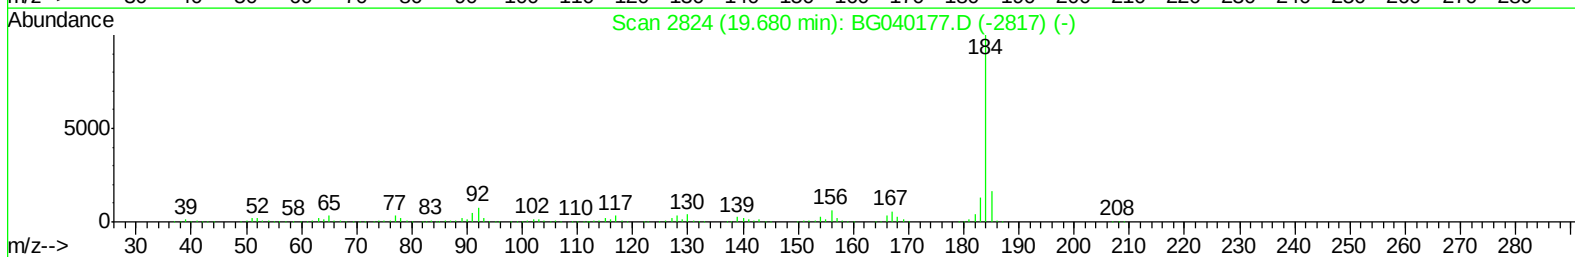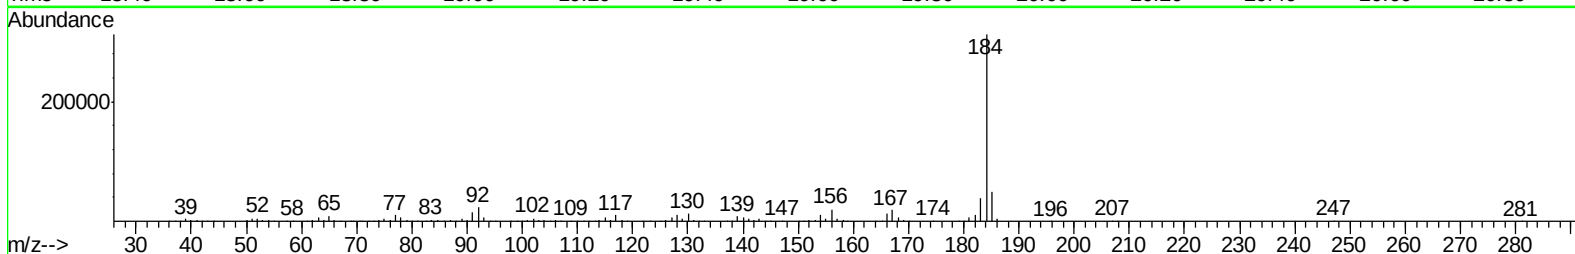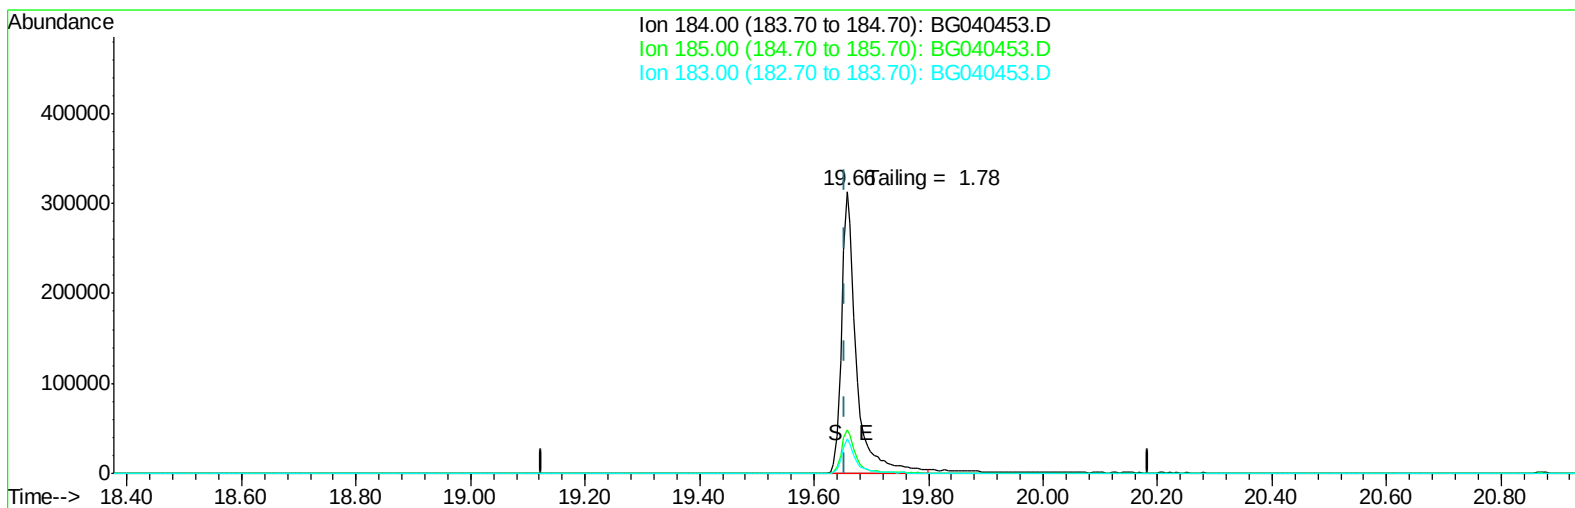

TIC: BG040453.D

(77) Benzidine

19.657min (+0.003) 220798.21ng

response 566102

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	15.57
183.00	12.90	12.08
0.00	0.00	0.00