
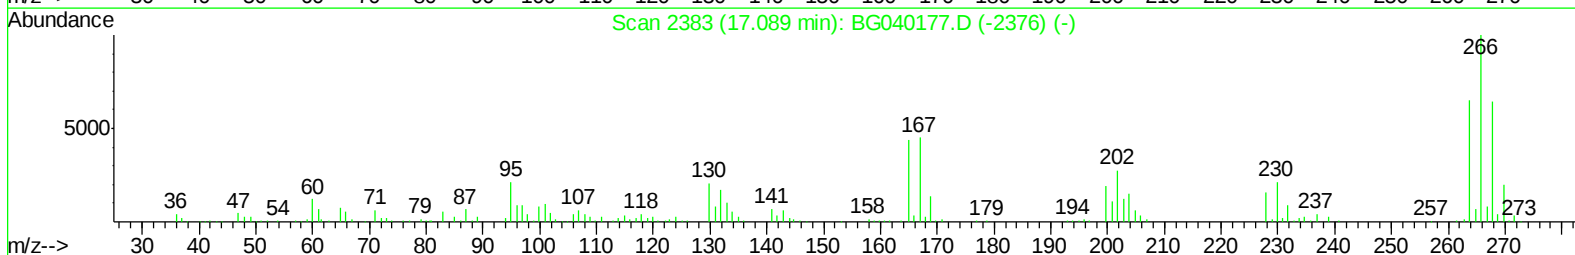
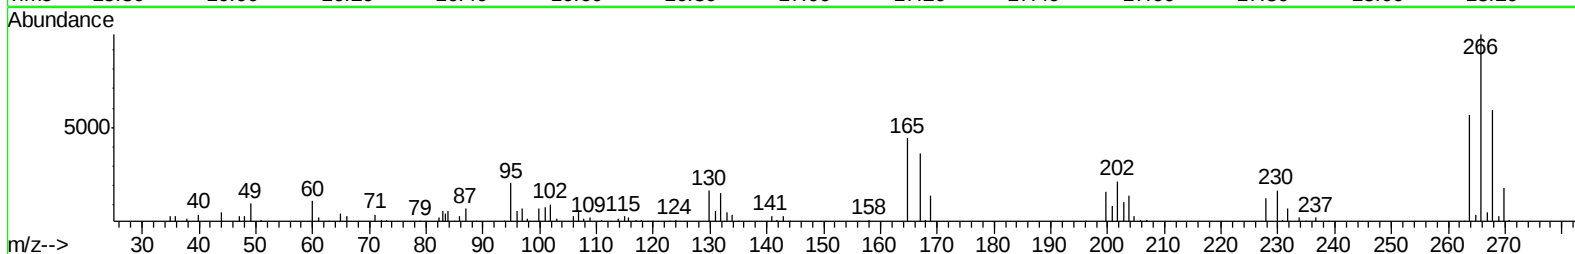


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041219\
Data File : BG040471.D
Acq On : 12 Apr 2019 21:31
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 05:27:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 00:33:11 2019
Response via : Initial Calibration

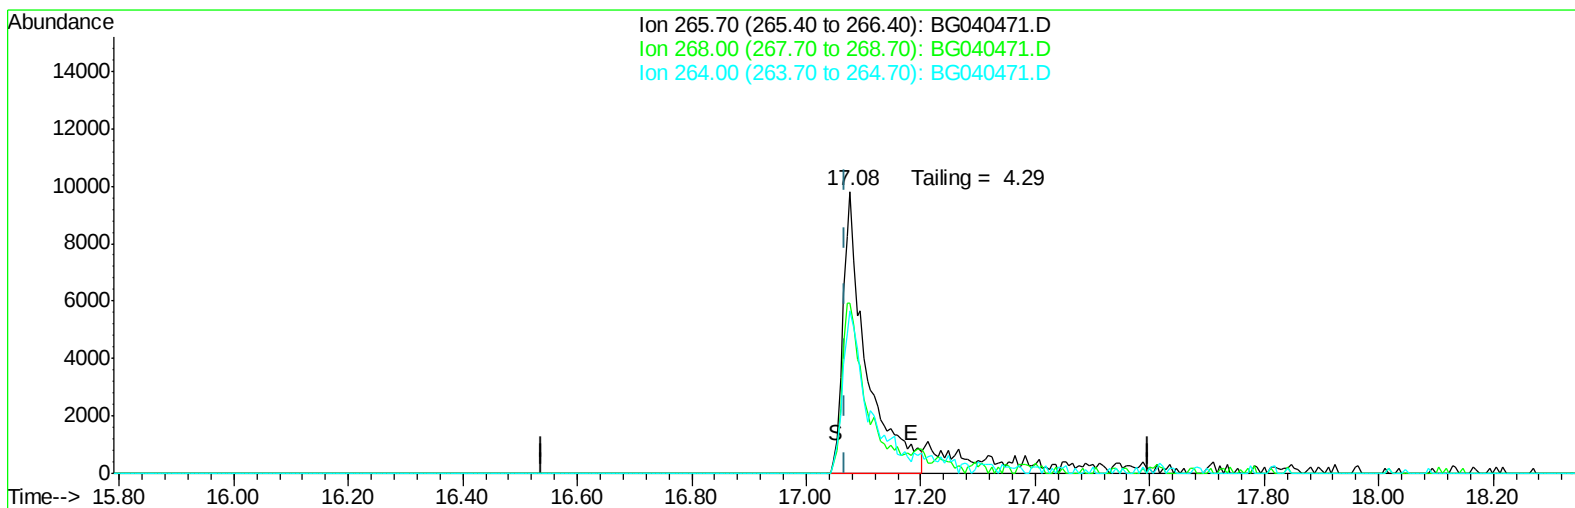

TIC: BG040471.D

(70) Pentachlorophenol (C)




17.077min (+0.008) 8635.19ng

response 27792

Ion	Exp%	Act%
265.70	100	100
268.00	68.70	60.57
264.00	64.80	57.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041219\
 Data File : BG040471.D
 Acq On : 12 Apr 2019 21:31
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 05:27:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 13 00:33:11 2019
 Response via : Initial Calibration

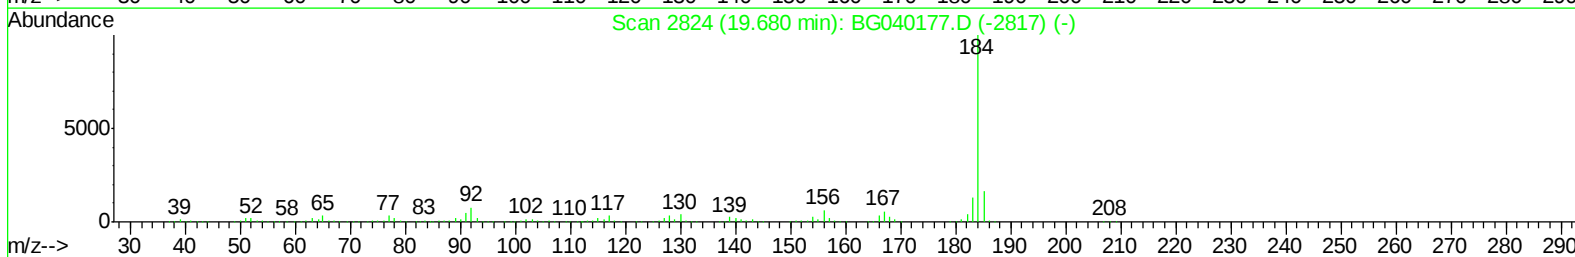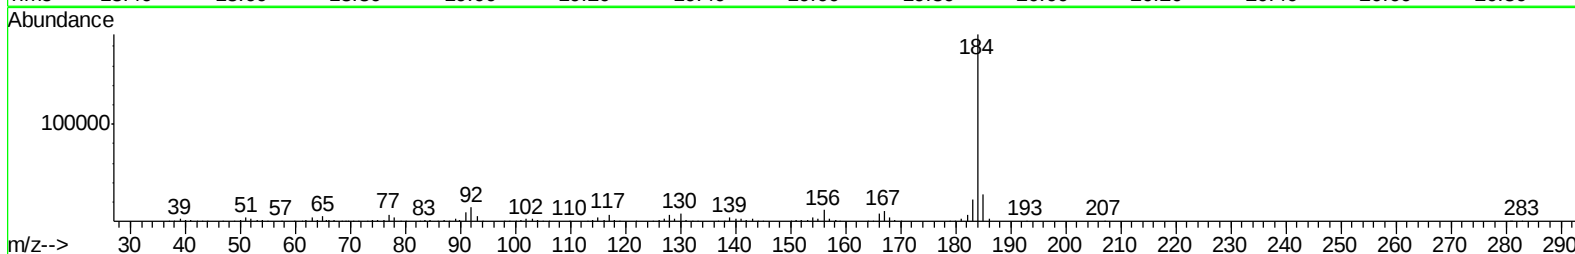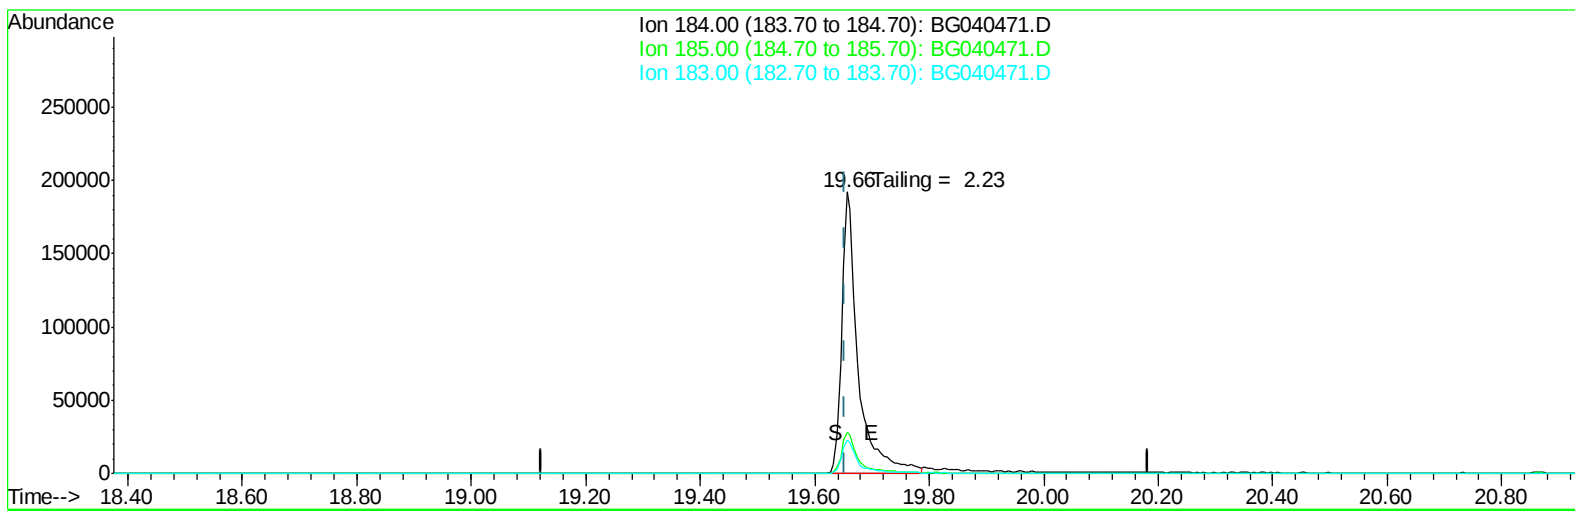

TIC: BG040471.D

(77) Benzidine

19.656min (+0.002) 0.00ng

response 383138

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	14.60
183.00	12.90	11.91
0.00	0.00	0.00