
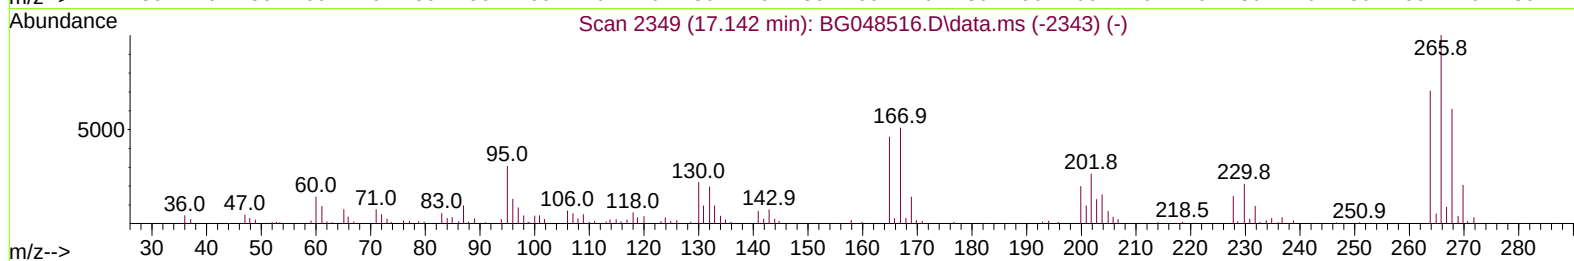
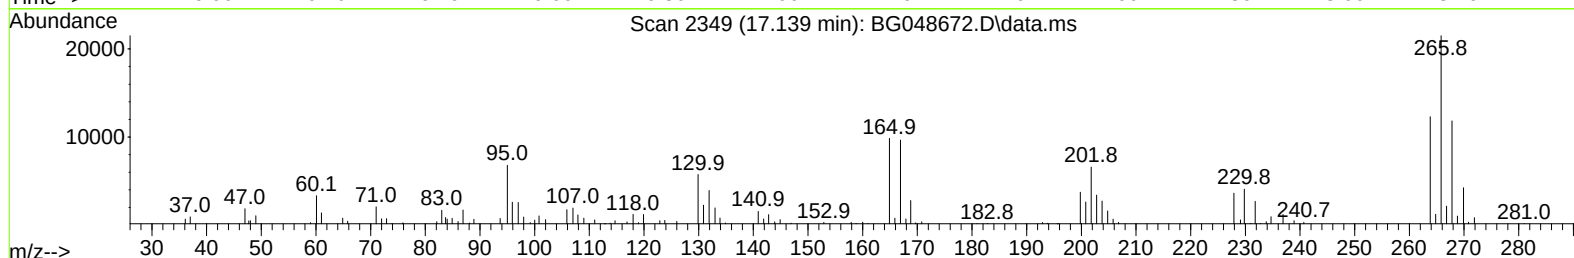


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041321\
Data File : BG048672.D
Acq On : 13 Apr 2021 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 02:05:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

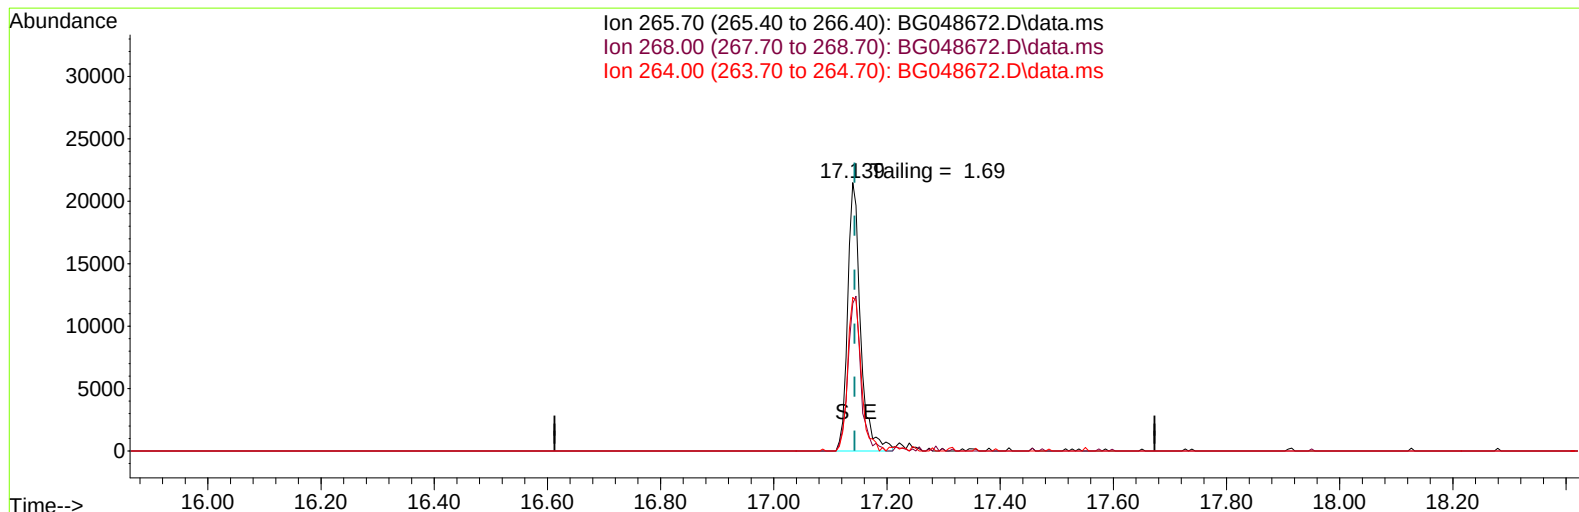

TIC: BG048672.D\data.ms

(70) Pentachlorophenol (C)




17.139min (-0.003) 56321.31 ng

response 34036

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	55.02
264.00	70.50	57.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041321\
Data File : BG048672.D
Acq On : 13 Apr 2021 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 02:05:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

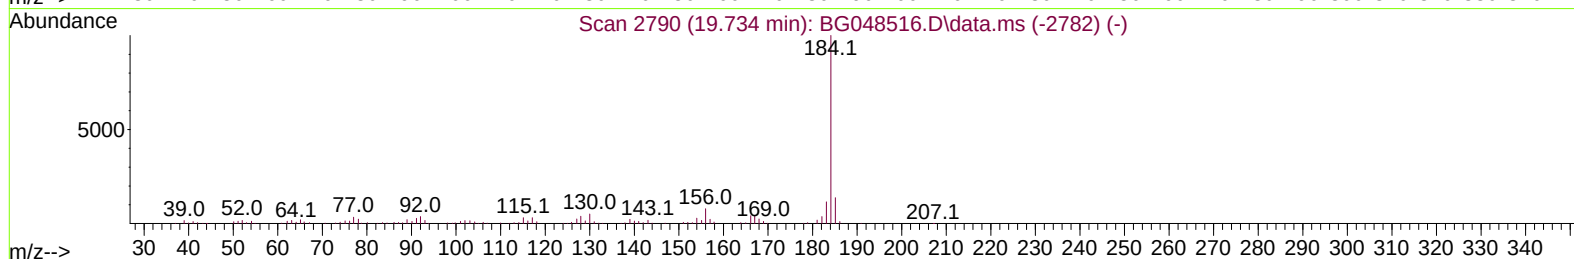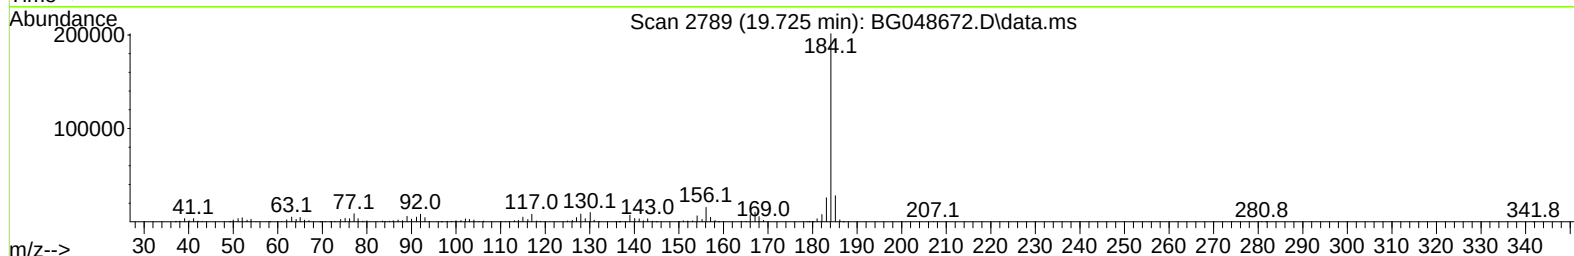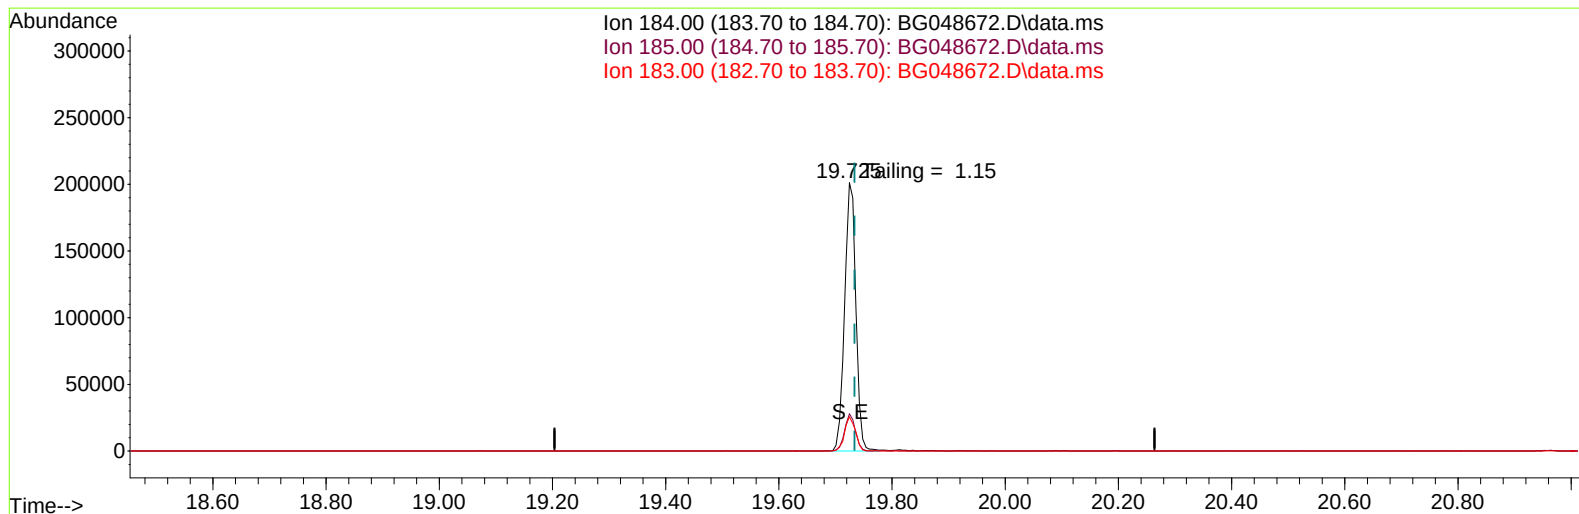

TIC: BG048672.D\data.ms

(77) Benzidine**19.725min (-0.009) 122471.48 ng****response 277866**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.92
183.00	11.50	12.80
0.00	0.00	0.00