
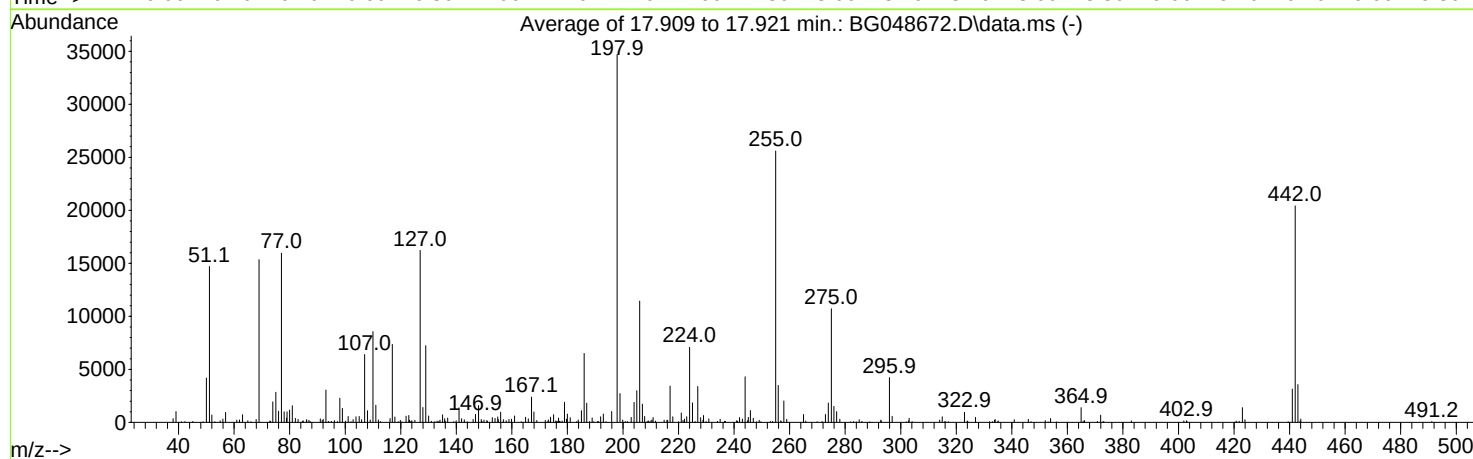


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041321\
 Data File : BG048672.D
 Acq On : 13 Apr 2021 12:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 07 10:06:00 2021

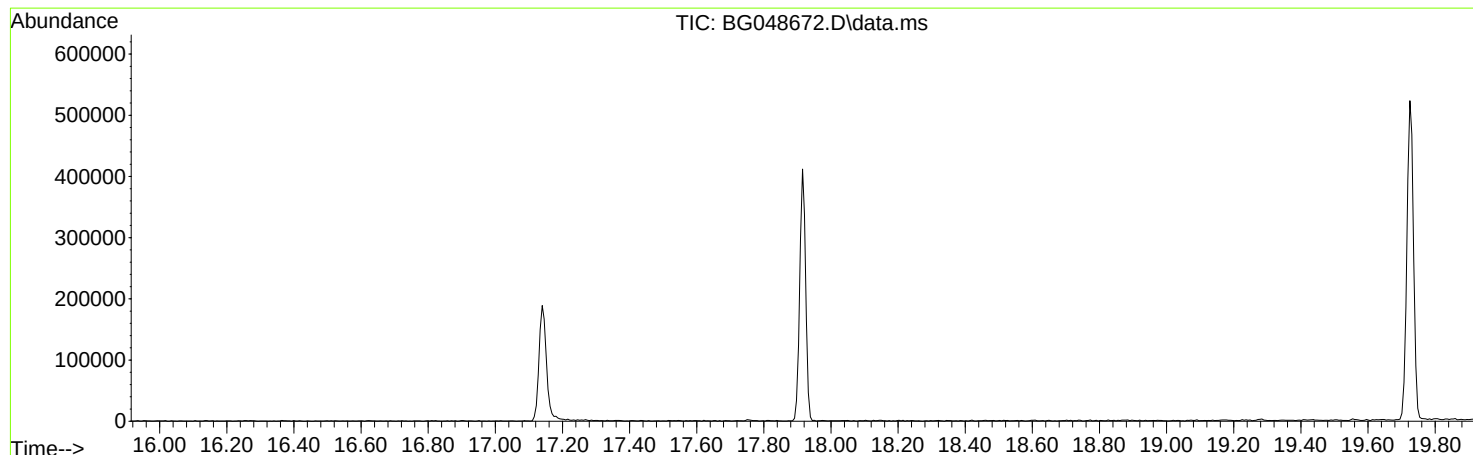

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	14699	PASS
68	69	0.00	2	1.7	267	PASS
69	198	0.00	100	44.2	15346	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	16220	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34701	PASS
199	198	5	9	7.8	2720	PASS
275	198	10	60	30.9	10714	PASS
365	198	1	100	4.0	1395	PASS
441	198	0.01	100	9.0	3138	PASS
442	198	50	100	58.8	20418	PASS
443	442	15	24	17.4	3558	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/13/2021	BNA_G	<u>BG048672.D</u>
Compound Name	Response	Retention Time
DDT	136517	20.959
DDD	1054	20.571
DDE	173	20.013
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1227	137744	0.89

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041321\
 Data File : BG048672.D
 Acq On : 13 Apr 2021 12:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 14 02:05:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 07 10:06:00 2021
 Response via : Initial Calibration

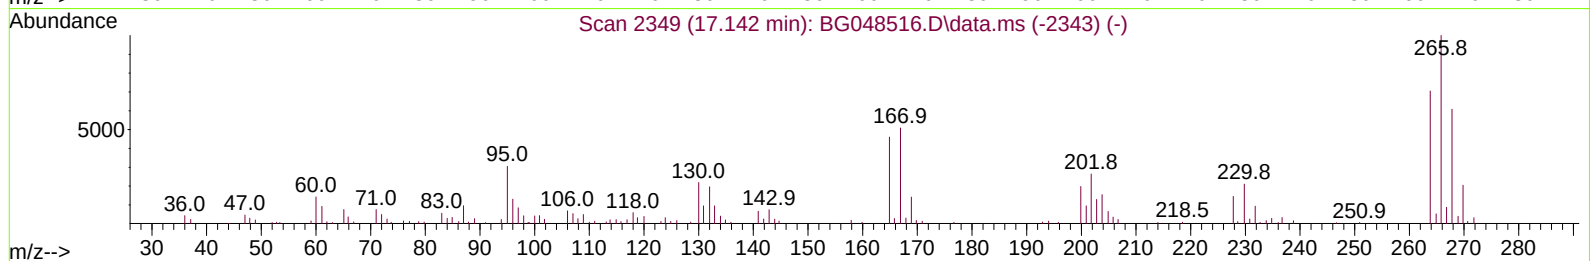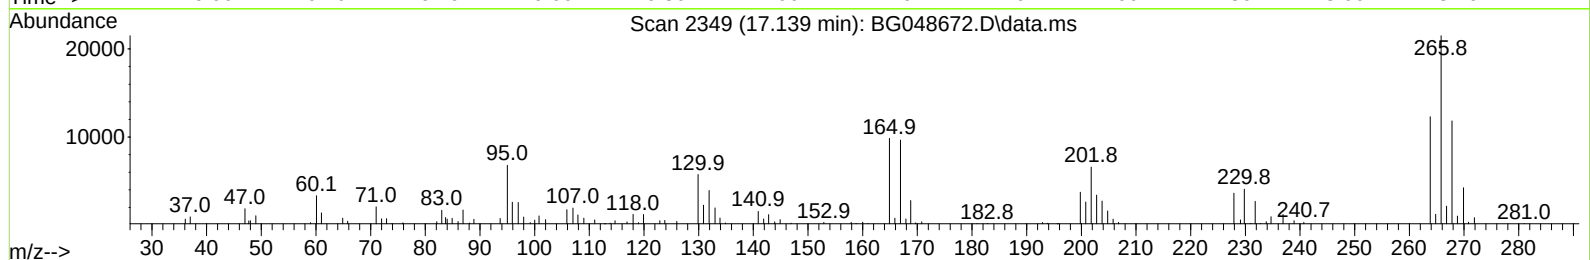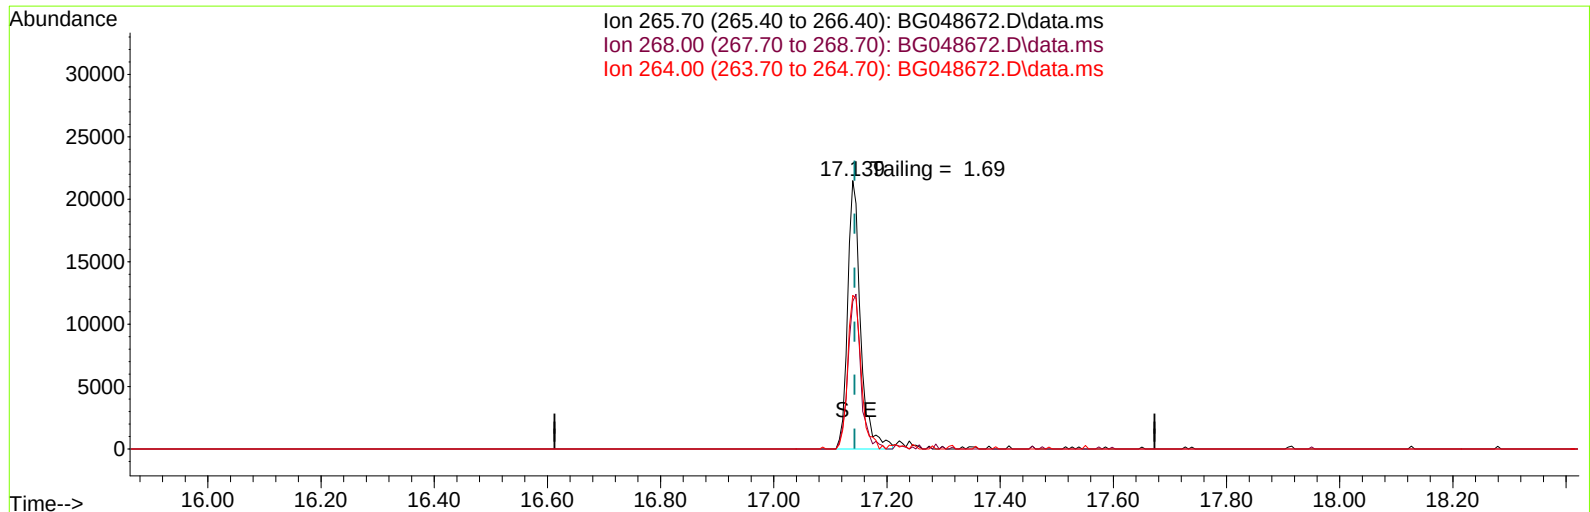

TIC: BG048672.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.003) 56321.31 ng




response 34036

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	55.02
264.00	70.50	57.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041321\
Data File : BG048672.D
Acq On : 13 Apr 2021 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 14 02:05:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 07 10:06:00 2021
Response via : Initial Calibration

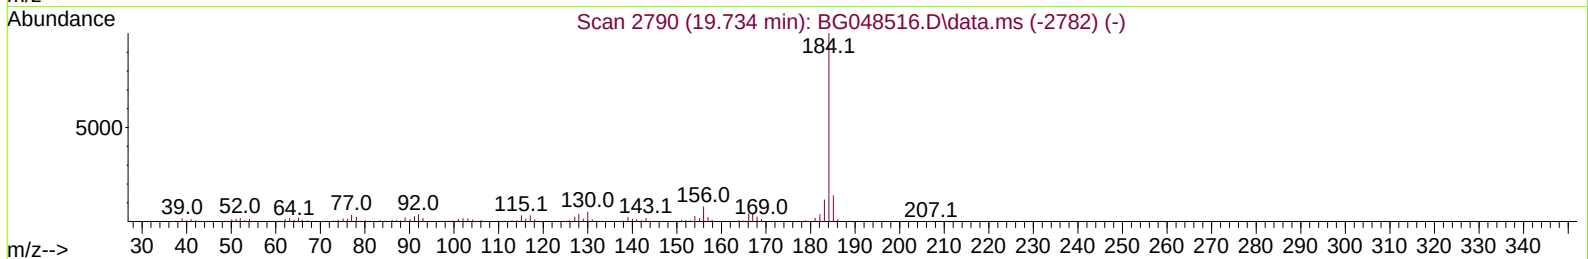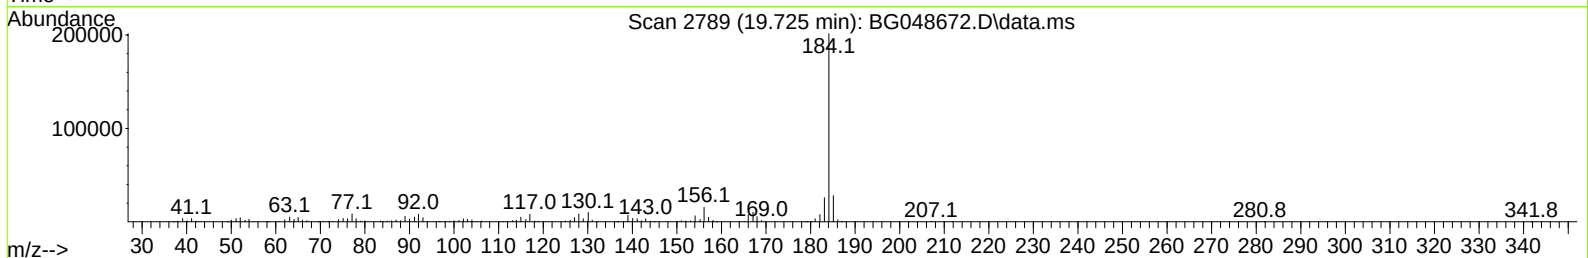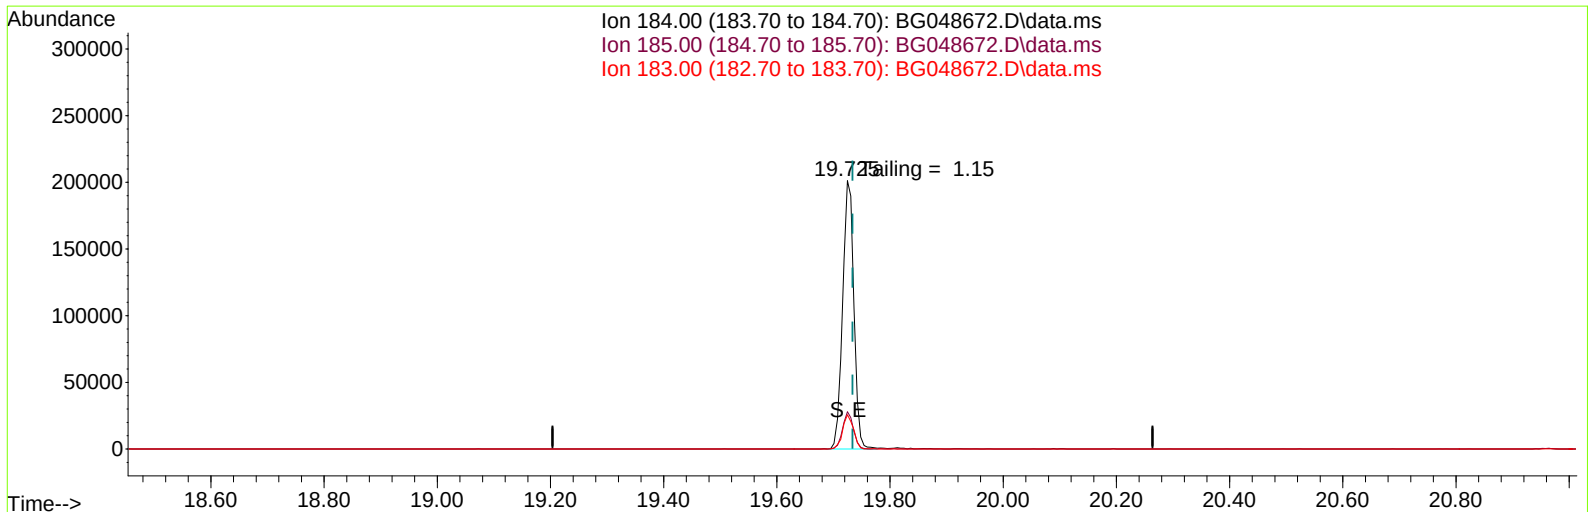

TIC: BG048672.D\data.ms

(77) Benzidine

19.725min (-0.009) 122471.48 ng

response 277866

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.92
183.00	11.50	12.80
0.00	0.00	0.00