


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041423\
Data File : BG057093.D
Acq On : 14 Apr 2023 9:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 13 05:15:23 2023

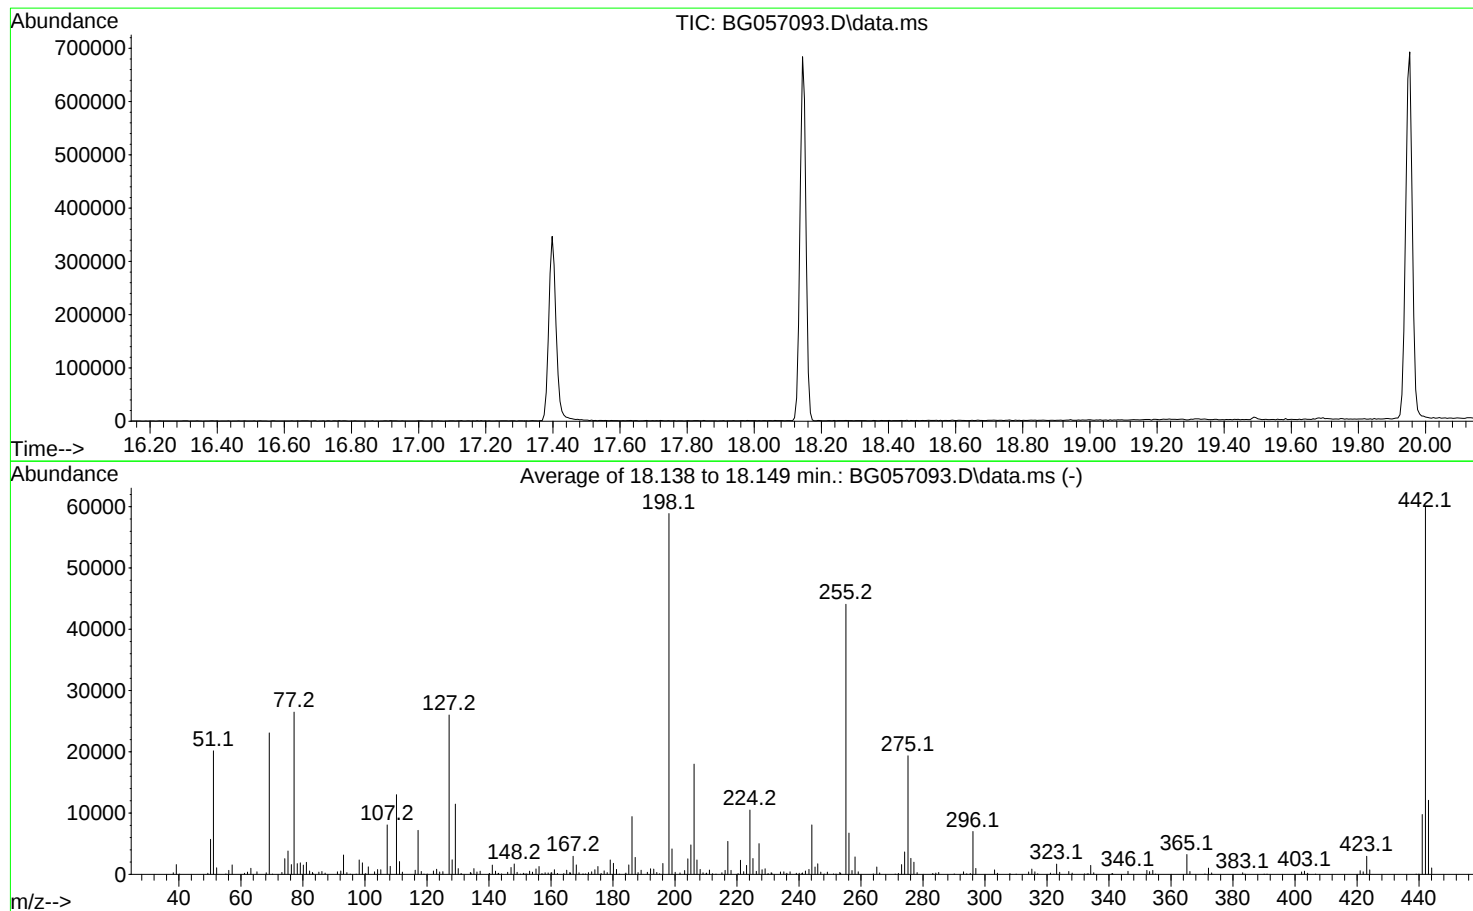

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	20163	PASS
68	69	0.00	2	1.1	251	PASS
69	198	0.00	100	39.2	23093	PASS
70	69	0.00	2	0.3	61	PASS
127	198	10	80	44.2	26013	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58877	PASS
199	198	5	9	7.1	4155	PASS
275	198	10	60	32.8	19340	PASS
365	198	1	100	5.5	3239	PASS
441	198	0.01	100	16.6	9767	PASS
442	442	50	100	100.0	60037	PASS
443	442	15	24	20.1	12092	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/14/2023	BNA_G	BG057093.D
Compound Name	Response	Retention Time
DDT	198249	21.192
DDD	4986	20.728
DDE	58	20.217
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5044	203293	2.48

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041423\
Data File : BG057093.D
Acq On : 14 Apr 2023 9:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 14 12:26:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:15:23 2023
Response via : Initial Calibration

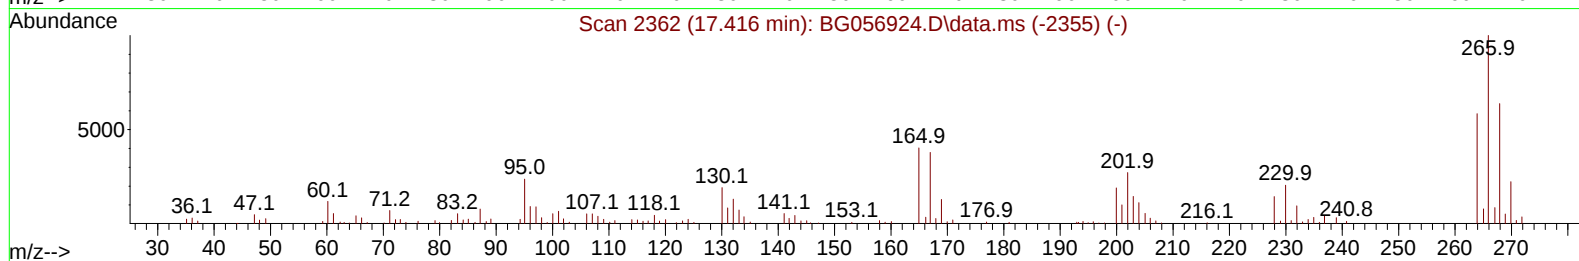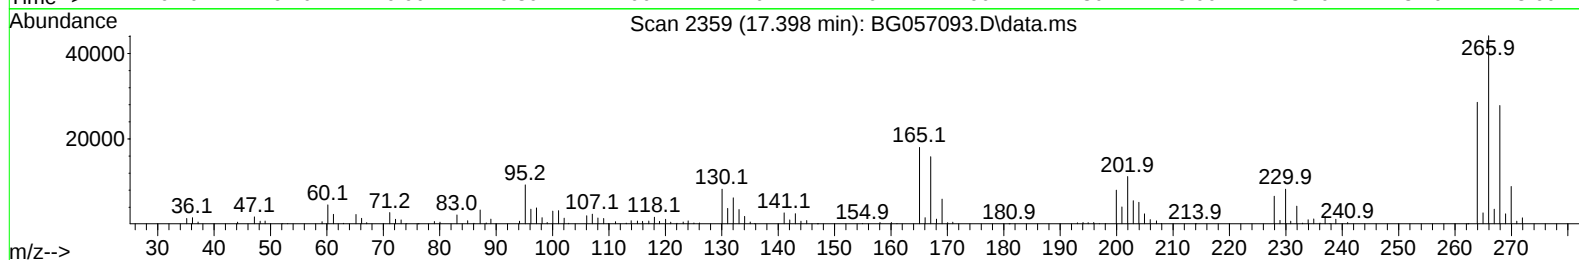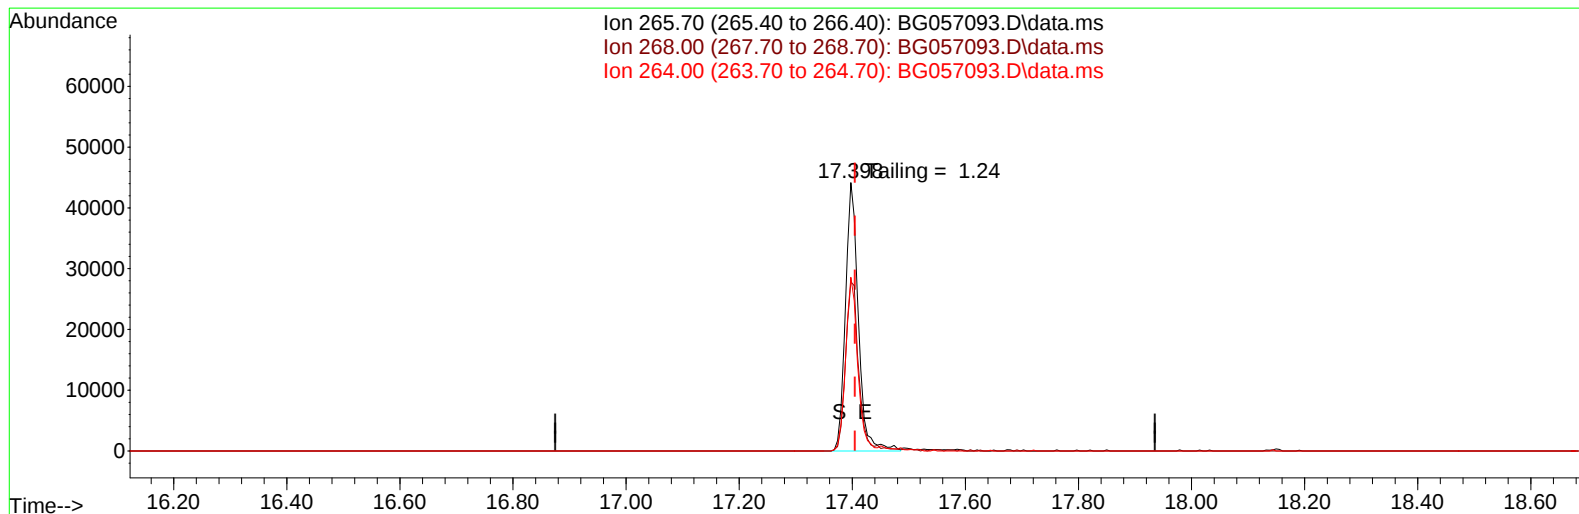

TIC: BG057093.D\data.ms

(70) Pentachlorophenol (C)

17.398min (-0.007) 26012.22 ng




response 70083

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.00
264.00	58.50	64.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041423\
Data File : BG057093.D
Acq On : 14 Apr 2023 9:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 14 12:26:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 05:15:23 2023
Response via : Initial Calibration

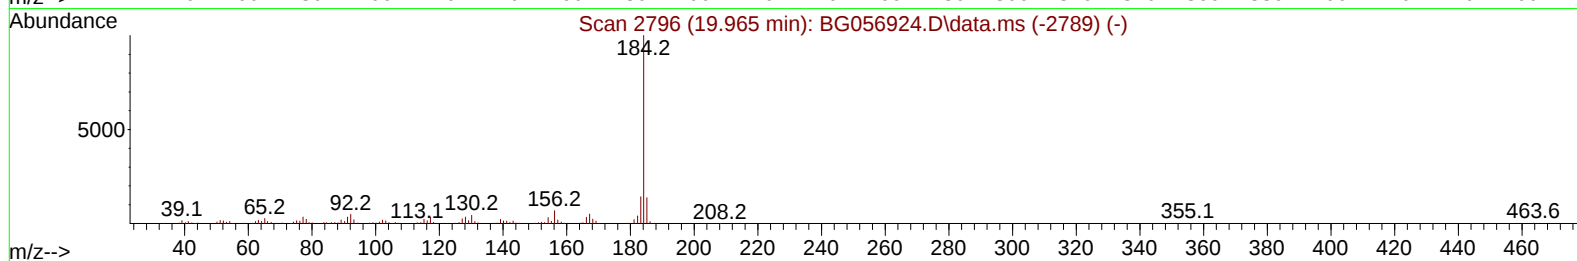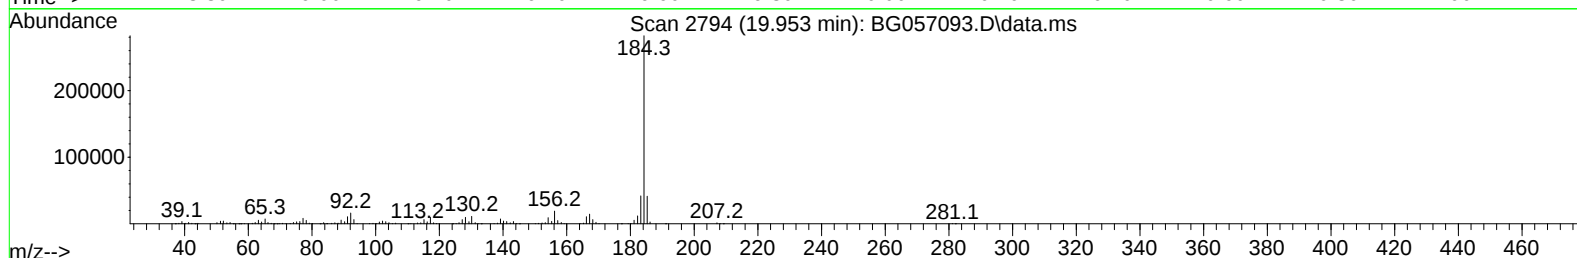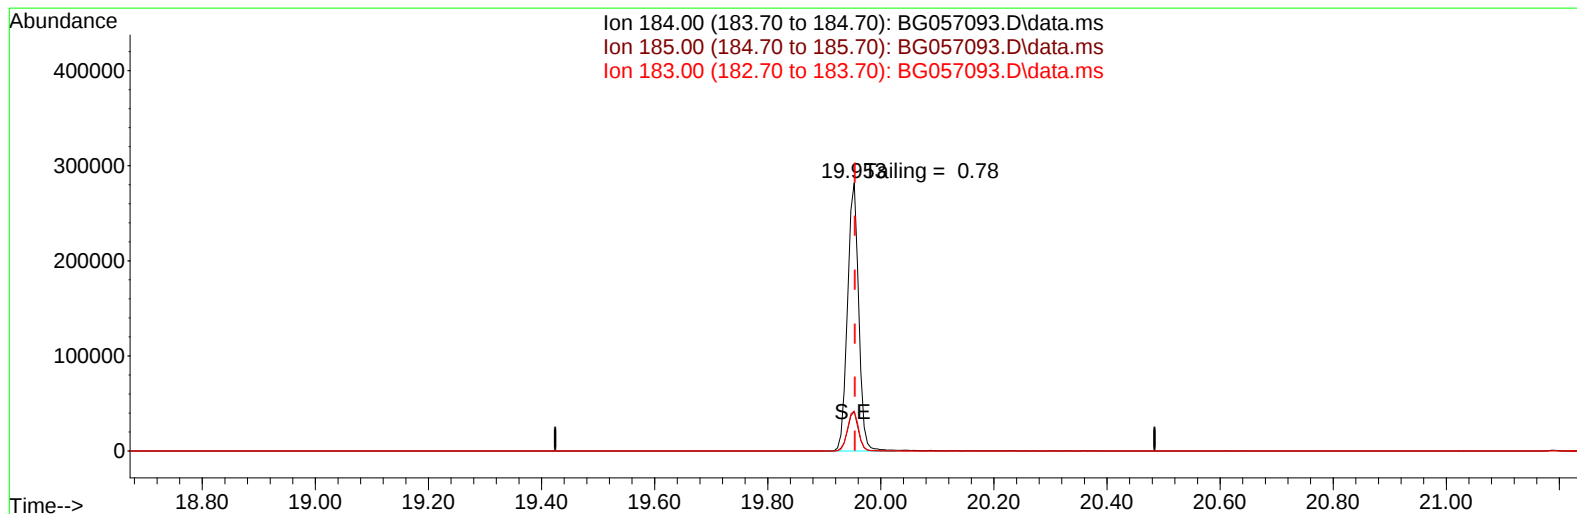

TIC: BG057093.D\data.ms

(77) Benzidine

19.953min (-0.002) 0.00 ng

response 388537

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.68
183.00	14.20	14.90
0.00	0.00	0.00