
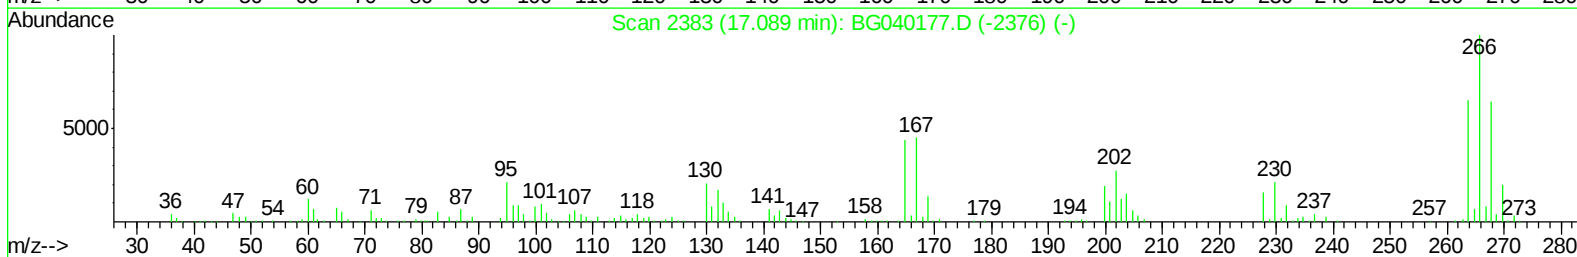
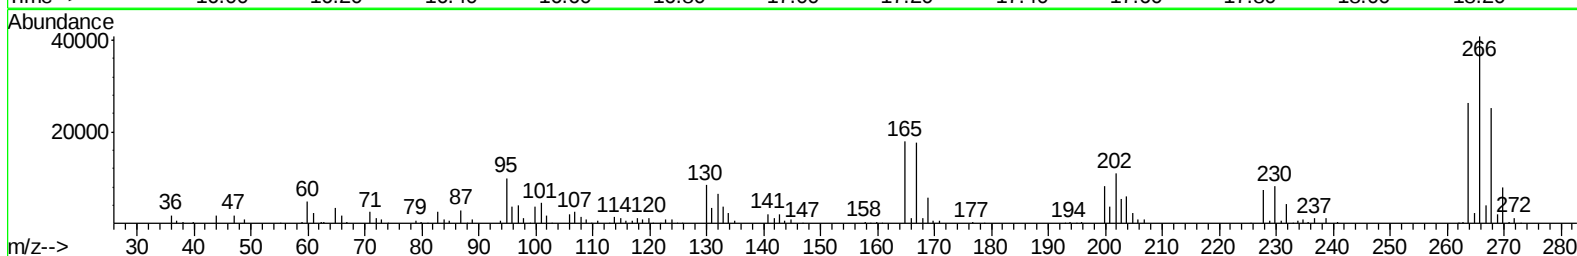


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041519\
Data File : BG040476.D
Acq On : 15 Apr 2019 12:17
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 15 13:07:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

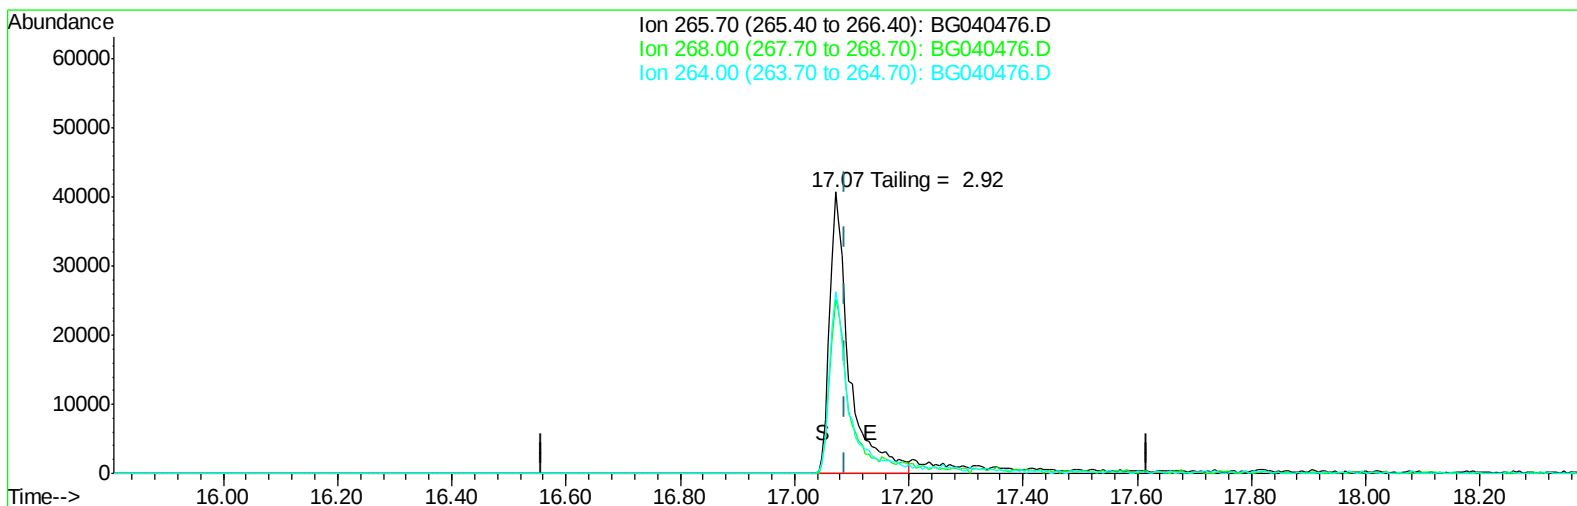

TIC: BG040476.D

(70) Pentachlorophenol (C)

17.071min (-0.017) 274973.19ng




response 97133

Ion	Exp%	Act%
265.70	100	100
268.00	68.70	61.72
264.00	64.80	64.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041519\
 Data File : BG040476.D
 Acq On : 15 Apr 2019 12:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 15 13:07:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

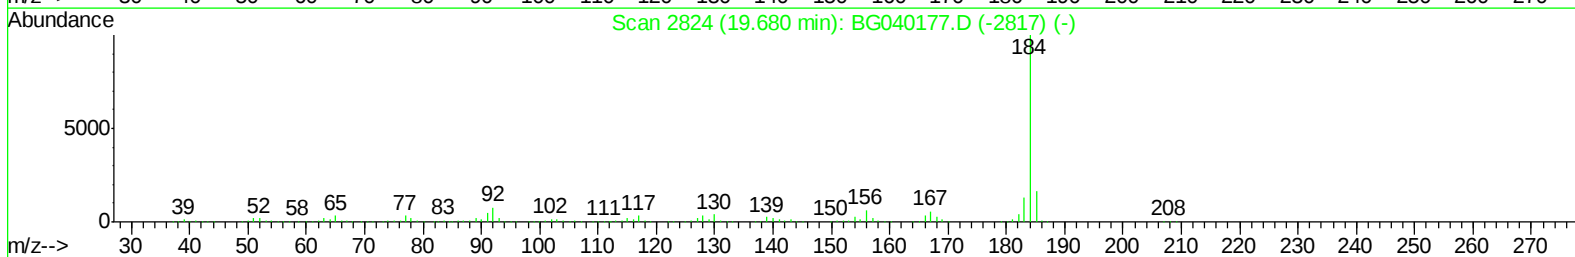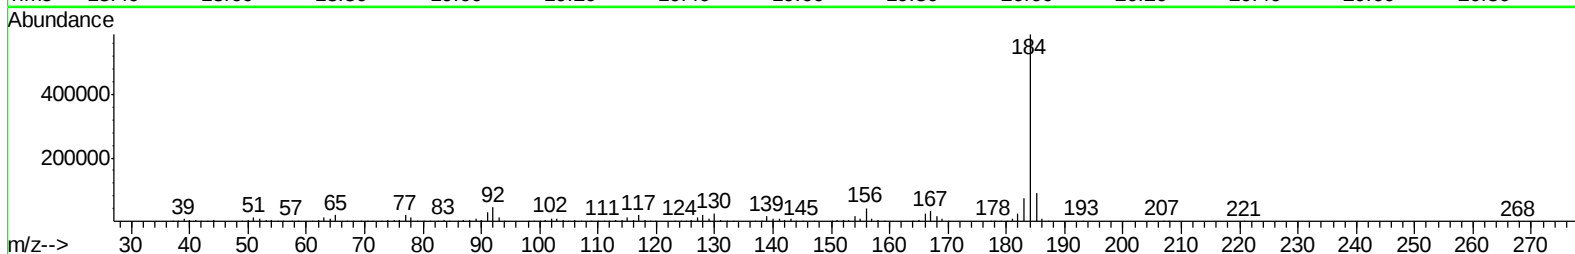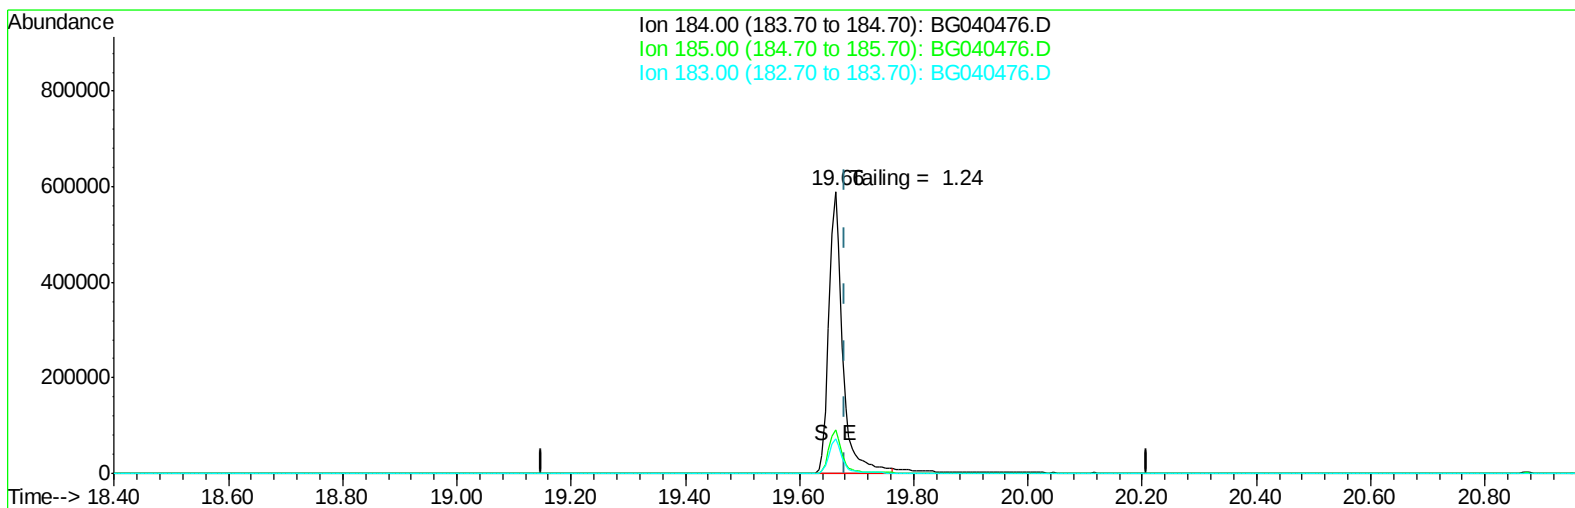

TIC: BG040476.D

(77) Benzidine

19.662min (-0.017) 0.00ng

response 1022248

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	15.36
183.00	12.90	12.09
0.00	0.00	0.00