
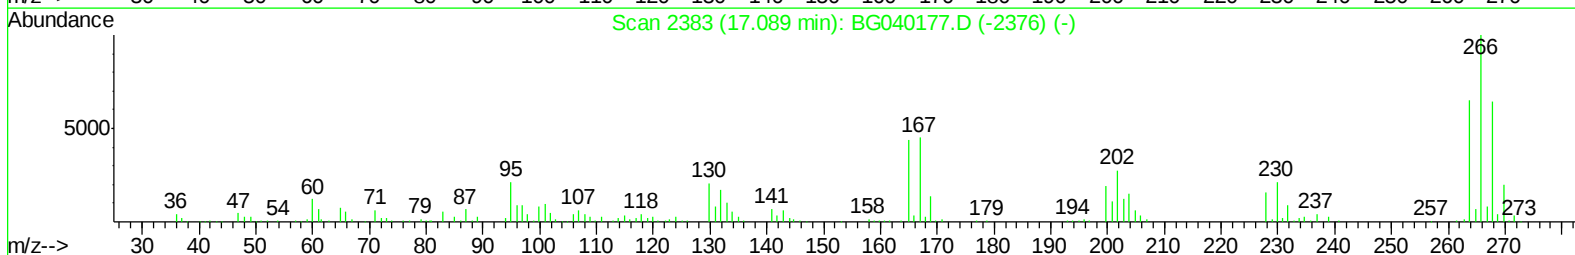
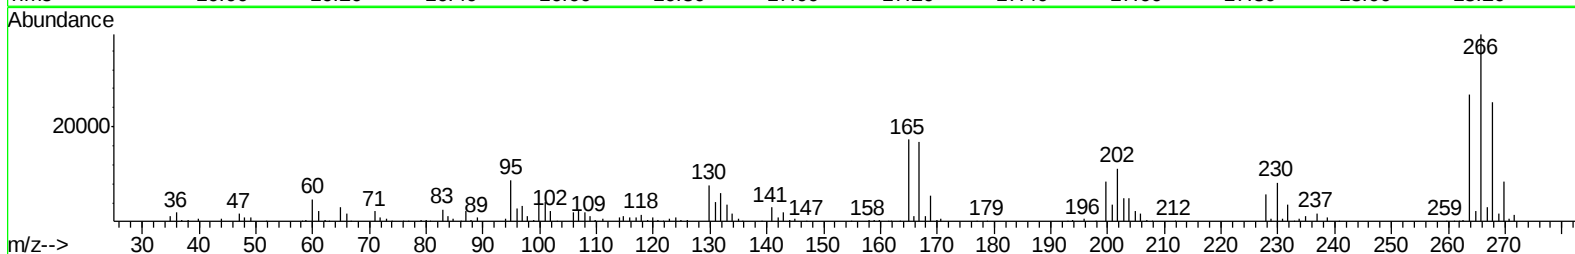


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041519\
Data File : BG040494.D
Acq On : 16 Apr 2019 00:20
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 05:33:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

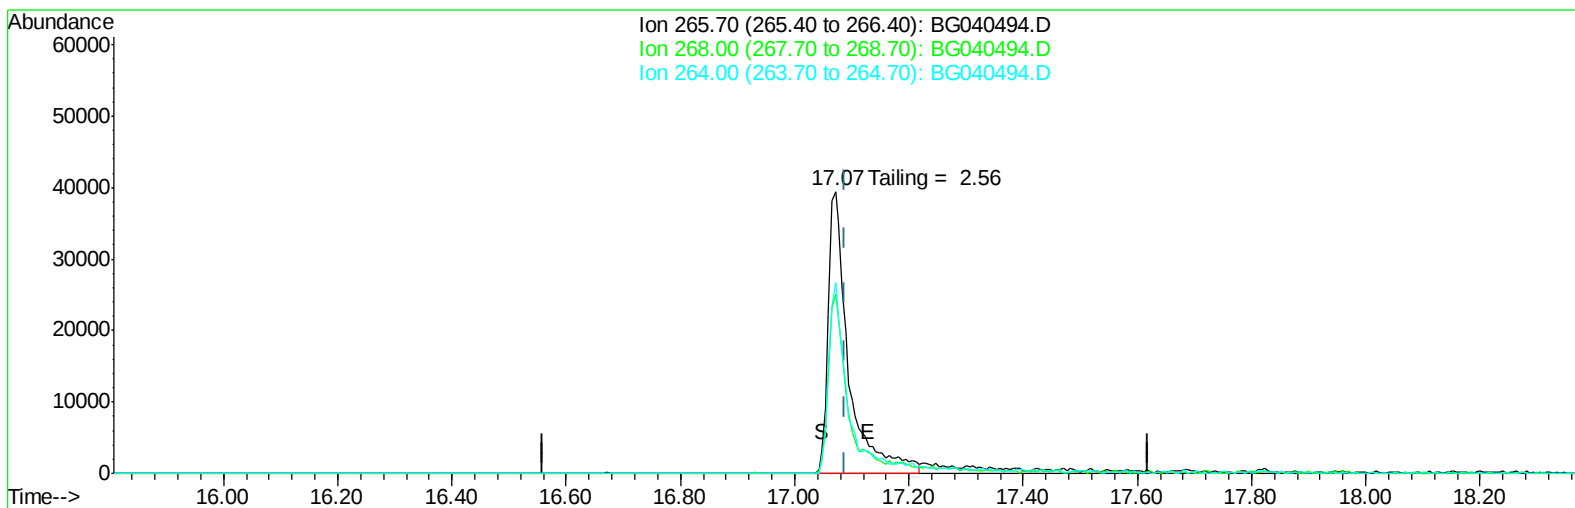

TIC: BG040494.D

(70) Pentachlorophenol (C)




17.071min (-0.018) 211029.24ng

response 98013

Ion	Exp%	Act%
265.70	100	100
268.00	68.70	63.77
264.00	64.80	67.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG041519\
 Data File : BG040494.D
 Acq On : 16 Apr 2019 00:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 05:33:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

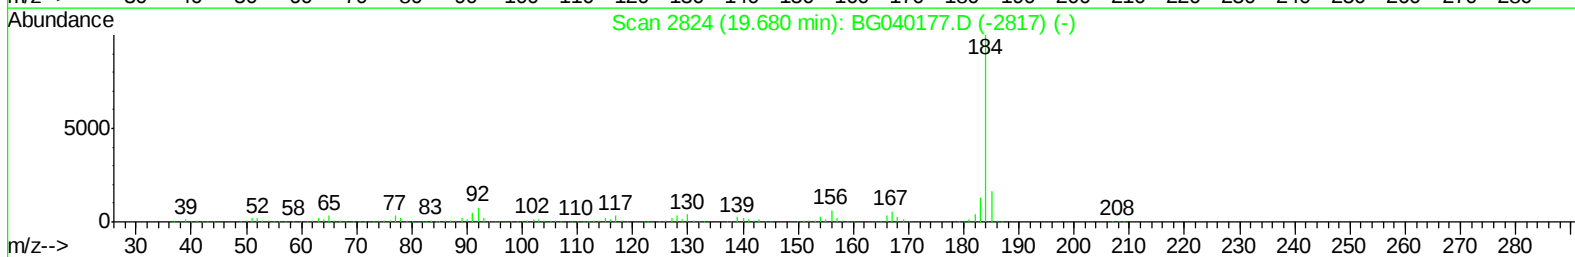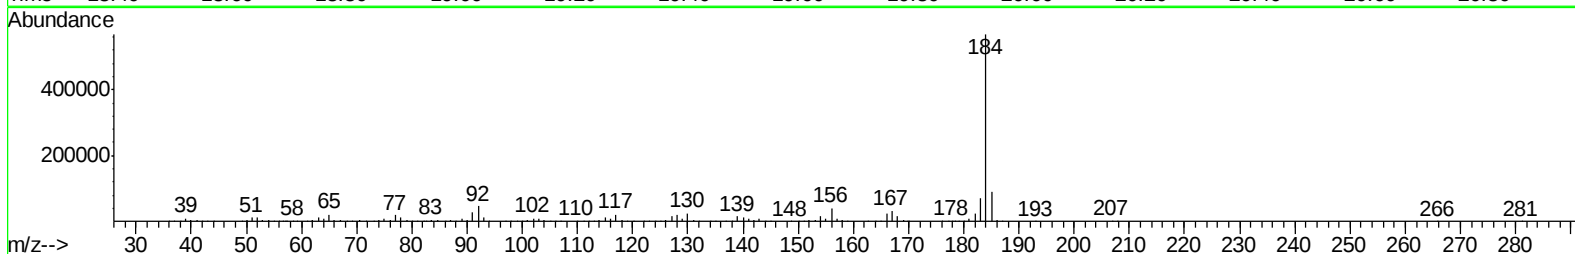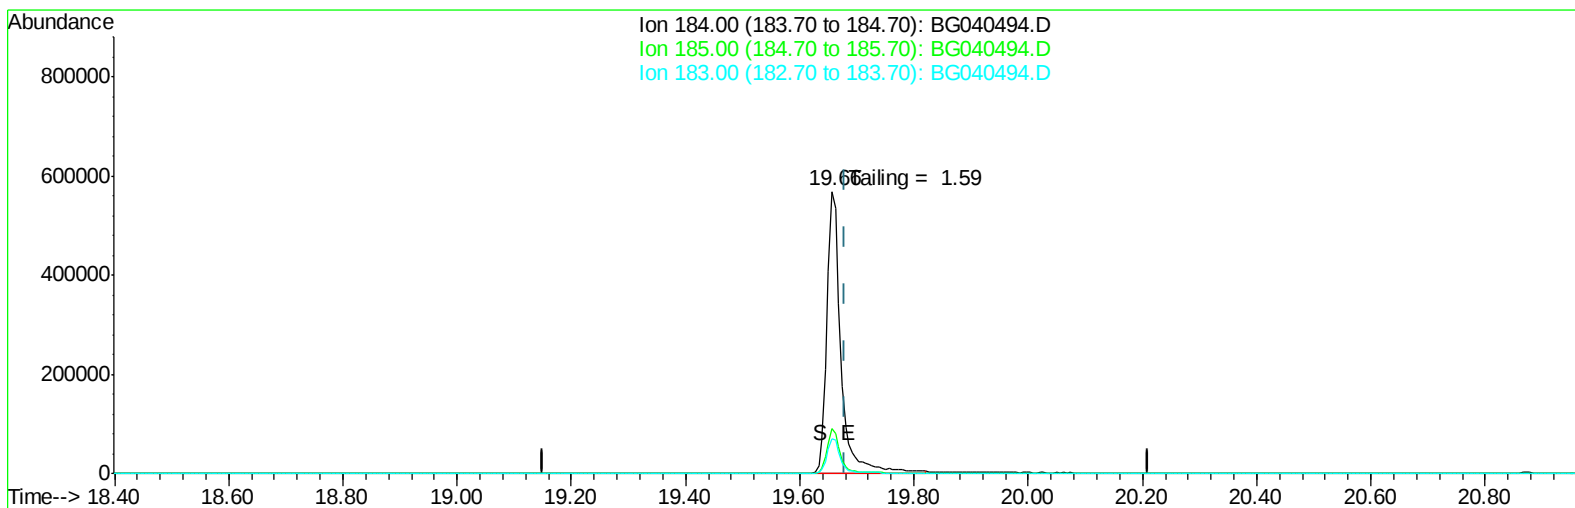

TIC: BG040494.D

(77) Benzidine

19.656min (-0.024) 0.00ng

response 992077

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	16.05
183.00	12.90	12.15
0.00	0.00	0.00