

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041519\
 Data File : BG040481.D
 Acq On : 15 Apr 2019 15:38
 Operator : JU/SJ
 Sample : K2407-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-11-D

Quant Time: Apr 16 02:16:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	47199	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	182119	20.00	ng	-0.02
39) Acenaphthene-d10	14.68	164	114718	20.00	ng	-0.02
64) Phenanthrene-d10	17.42	188	308863	20.00	ng	-0.02
76) Chrysene-d12	21.69	240	321358	20.00	ng	-0.04
87) Perylene-d12	24.98	264	346918	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	415483	146.34	ng	-0.02
7) Phenol-d6	7.20	99	575063	146.56	ng	-0.02
23) Nitrobenzene-d5	9.22	82	343035	100.12	ng	-0.02
42) 2,4,6-Tribromophenol	16.17	330	205897	166.07	ng	-0.02
45) 2-Fluorobiphenyl	13.30	172	759544	98.11	ng	-0.02
79) Terphenyl-d14	20.03	244	1321672	92.52	ng	-0.02
Target Compounds						
50) Dimethylphthalate	14.13	163	86100	9.590	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041519\
Data File : BG040481.D
Acq On : 15 Apr 2019 15:38
Operator : JU/SJ
Sample : K2407-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-11-D

Quant Time: Apr 16 02:16:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

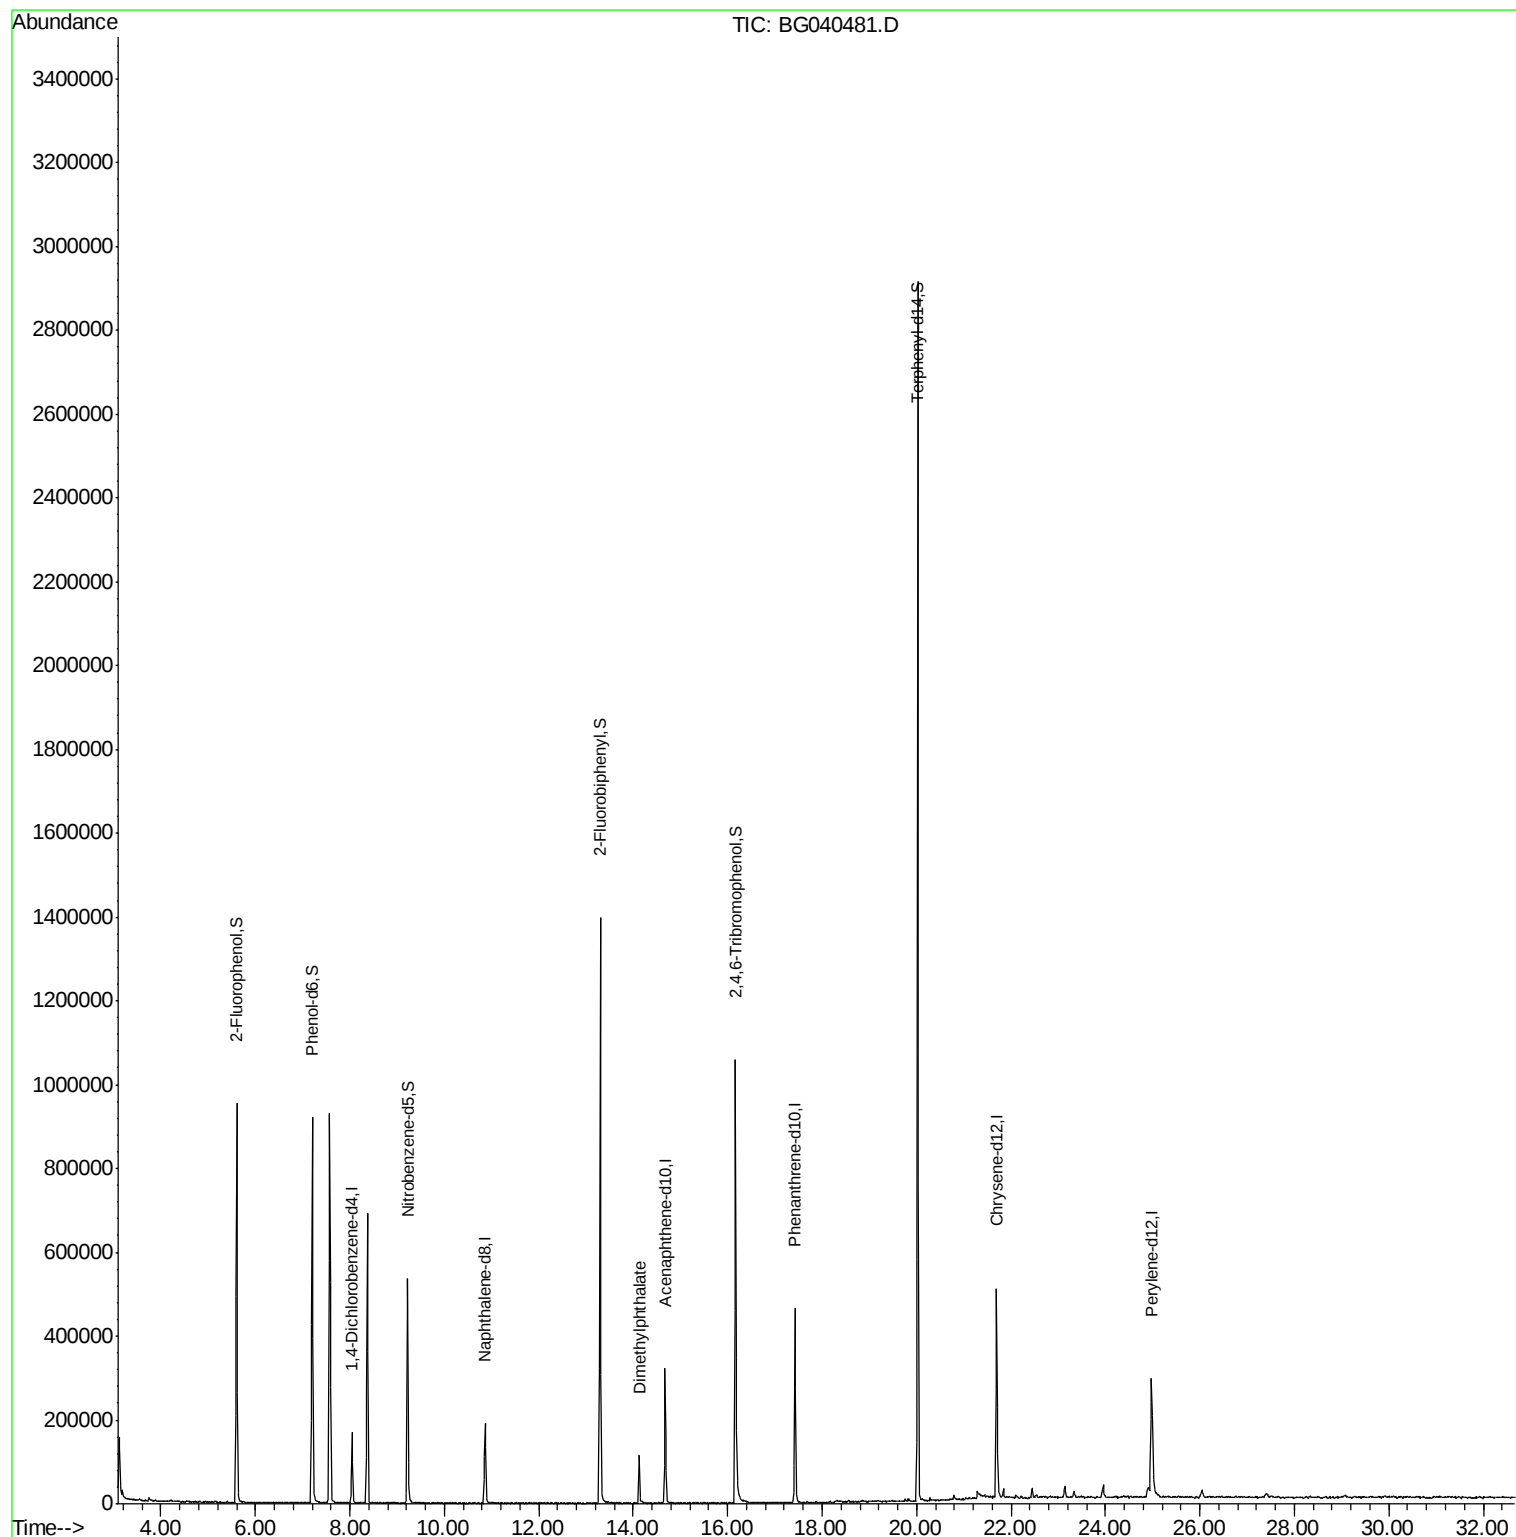




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 844
Delta R.T. -0.02 min
Lab File: BG040481.D
Acq: 15 Apr 2019 15:38

Instrument :
BNA_G
ClientSampleId :
TP-11-D

Tgt Ion:152 Resp: 47199
Ion Ratio Lower Upper
152 100
150 158.2 123.7 185.5
115 57.7 46.9 70.3

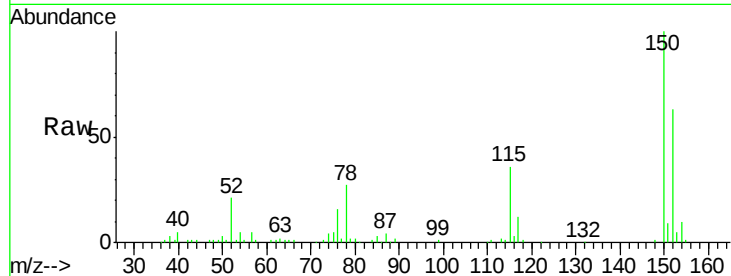


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

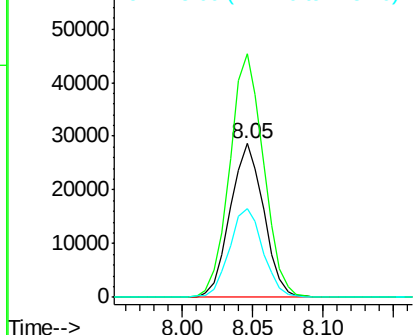



#5

2-Fluorophenol
Concen: 146.339 ng
RT: 5.60 min Scan# 428
Delta R.T. -0.02 min
Lab File: BG040481.D
Acq: 15 Apr 2019 15:38

Tgt Ion:112 Resp: 415483
Ion Ratio Lower Upper
112 100
64 70.2 54.2 81.2
63 33.7 26.4 39.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

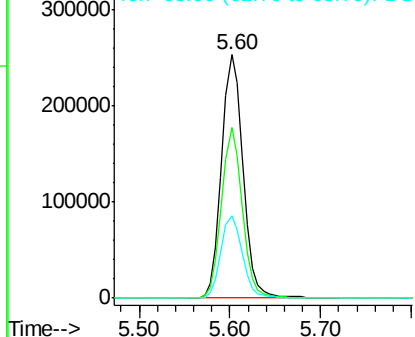



#7

Phenol-d6

Concen: 146.558 ng

RT: 7.20 min Scan# 700

Delta R.T. -0.02 min

Lab File: BG040481.D

Acq: 15 Apr 2019 15:38

Instrument :

BNA_G

ClientSampleId :

TP-11-D


Tgt Ion: 99 Resp: 575063

Ion Ratio Lower Upper



99 100

42 20.0 16.2 24.2

71 32.6 26.8 40.2

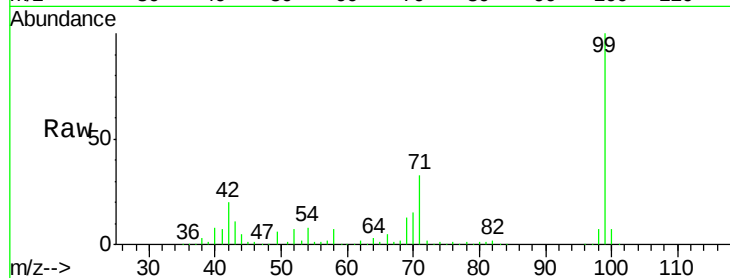

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

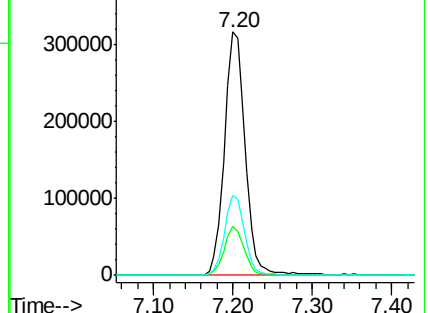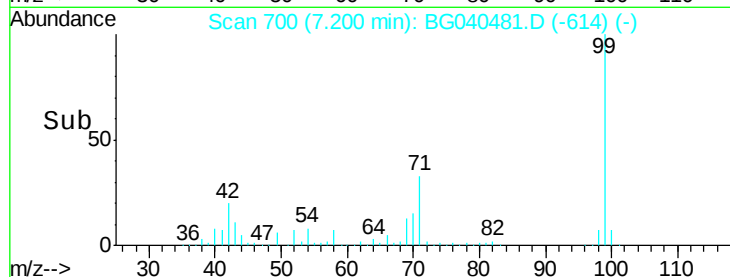

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BG040481.D

Acq: 15 Apr 2019 15:38

Tgt Ion: 136 Resp: 182119


Ion Ratio Lower Upper

136 100



137 10.1 8.9 13.3


54 9.8 9.6 14.4

68 7.5 5.1 7.7

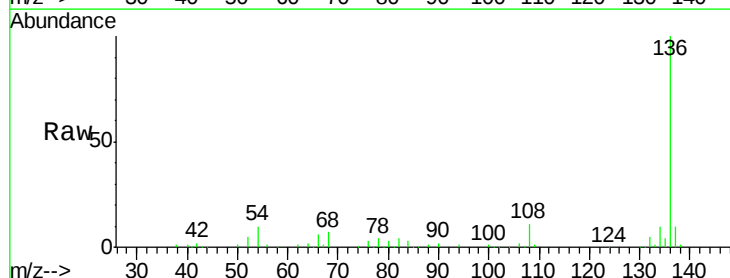

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



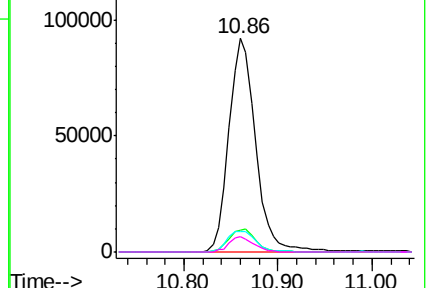
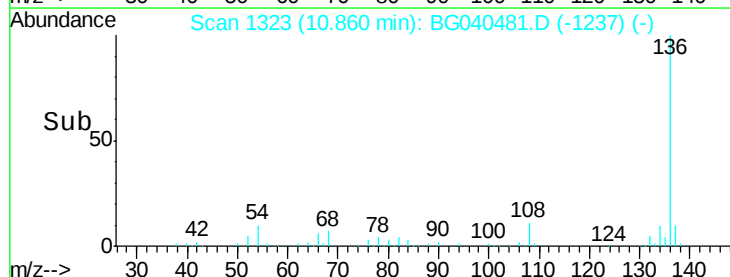


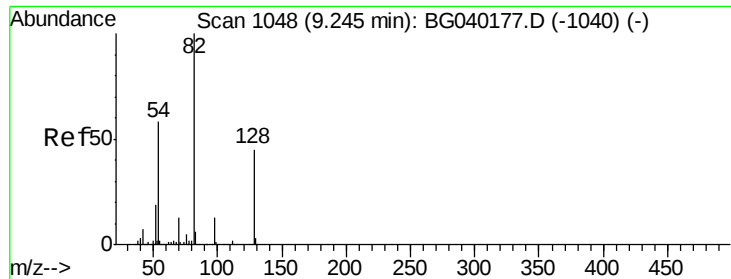

#23
Nitrobenzene-d5
Concen: 100.118 ng
RT: 9.22 min Scan# 1044
Delta R.T. -0.02 min
Lab File: BG040481.D
Acq: 15 Apr 2019 15:38




Instrument :
BNA_G
ClientSampleId :
TP-11-D

Tgt Ion: 82 Resp: 343035
Ion Ratio Lower Upper
82 100
128 42.3 35.8 53.8
54 53.4 46.2 69.2

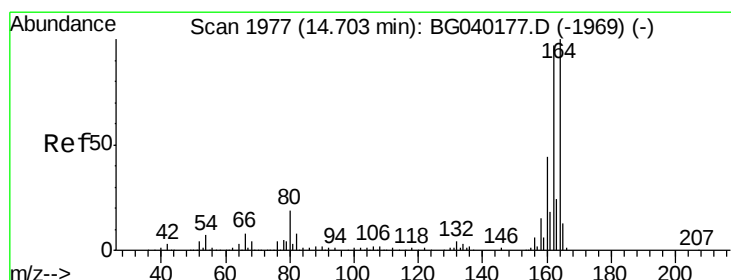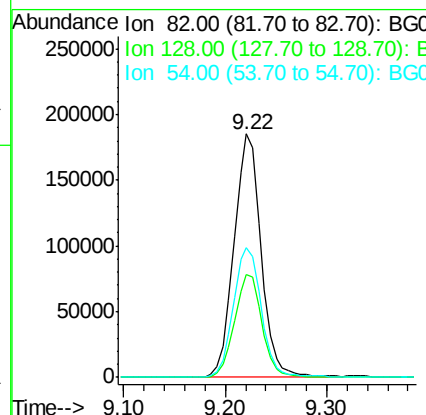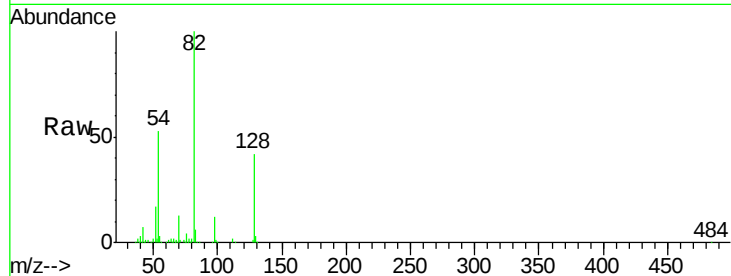

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1973
Delta R.T. -0.02 min
Lab File: BG040481.D
Acq: 15 Apr 2019 15:38

Tgt Ion: 164 Resp: 114718
Ion Ratio Lower Upper
164 100
162 99.0 77.4 116.2
160 47.4 35.3 52.9



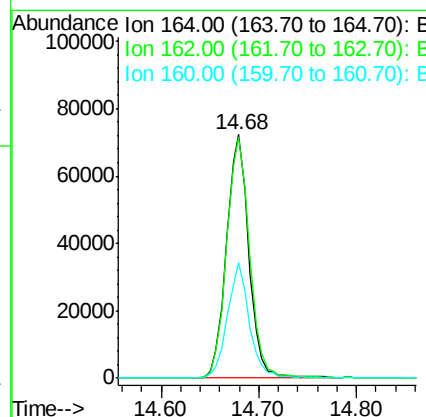





#42
 2,4,6-Tribromophenol
 Concen: 166.072 ng
 RT: 16.17 min Scan# 2226
 Delta R.T. -0.02 min
 Lab File: BG040481.D
 Acq: 15 Apr 2019 15:38




Instrument :
 BNA_G
 ClientSampleId :
 TP-11-D


Tgt Ion:330 Resp: 205897
 Ion Ratio Lower Upper
 330 100
 332 97.1 76.6 115.0
 141 41.0 32.6 48.8

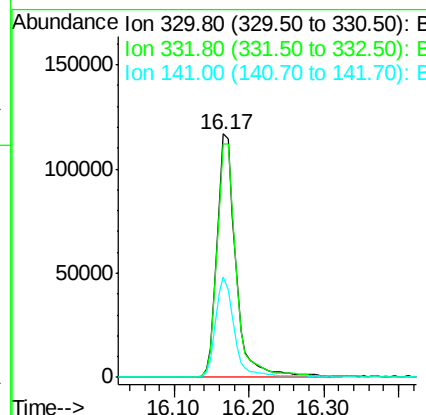

#45
 2-Fluorobiphenyl
 Concen: 98.107 ng
 RT: 13.30 min Scan# 1738
 Delta R.T. -0.02 min
 Lab File: BG040481.D
 Acq: 15 Apr 2019 15:38

Tgt Ion:172 Resp: 759544
 Ion Ratio Lower Upper
 172 100
 171 36.7 30.5 45.7
 170 24.3 20.1 30.1

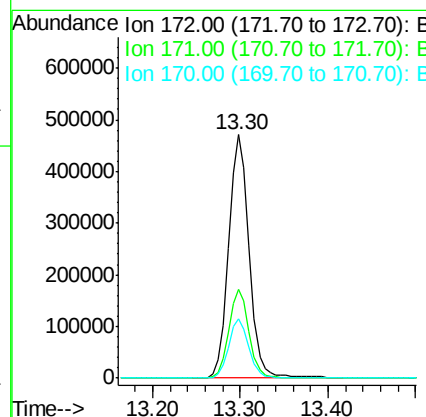



#50

Dimethylphthalate

Concen: 9.590 ng

RT: 14.13 min Scan# 1879

Delta R.T. -0.02 min

Lab File: BG040481.D

Acq: 15 Apr 2019 15:38

Instrument :

BNA_G

ClientSampleId :

TP-11-D


Tgt Ion:163 Resp: 86100

Ion Ratio Lower Upper

163 100

194 5.2 4.1 6.1




164 10.6 8.6 13.0



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

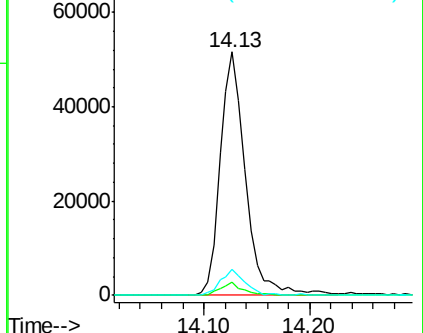

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2440

Delta R.T. -0.02 min

Lab File: BG040481.D

Acq: 15 Apr 2019 15:38


Tgt Ion:188 Resp: 308863

Ion Ratio Lower Upper

188 100

94 8.6 7.0 10.4



80 10.5 8.6 13.0




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG0

Ion 80.00 (79.70 to 80.70): BG0



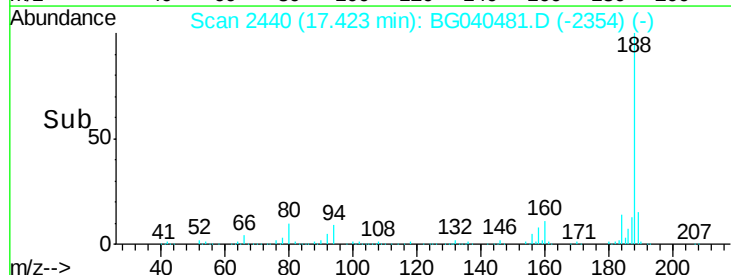
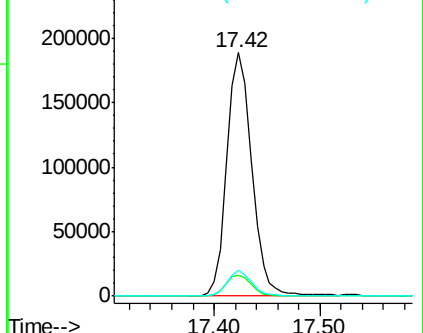


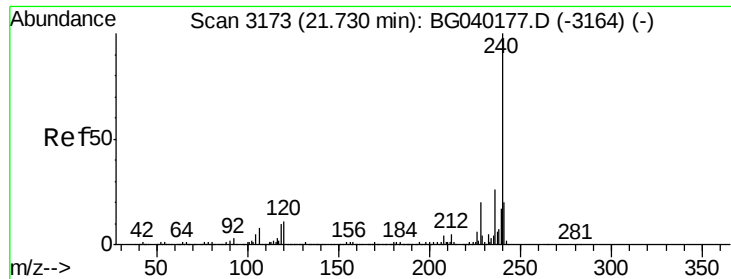

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.69 min Scan# 3167
Delta R.T. -0.04 min
Lab File: BG040481.D
Acq: 15 Apr 2019 15:38




Instrument :
BNA_G
ClientSampleId :
TP-11-D




Tgt Ion:240 Resp: 321358
Ion Ratio Lower Upper
240 100
120 11.6 8.4 12.6
236 26.3 20.8 31.2

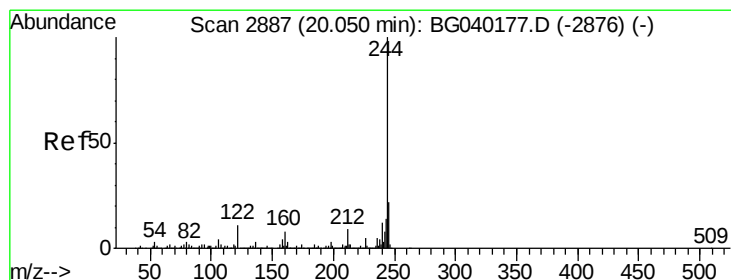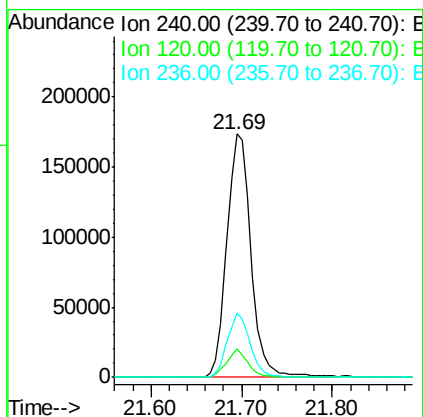

#79
Terphenyl-d14
Concen: 92.523 ng
RT: 20.03 min Scan# 2883
Delta R.T. -0.02 min
Lab File: BG040481.D
Acq: 15 Apr 2019 15:38

Tgt Ion:244 Resp: 1321672
Ion Ratio Lower Upper
244 100
212 9.0 7.0 10.6
122 11.3 8.5 12.7

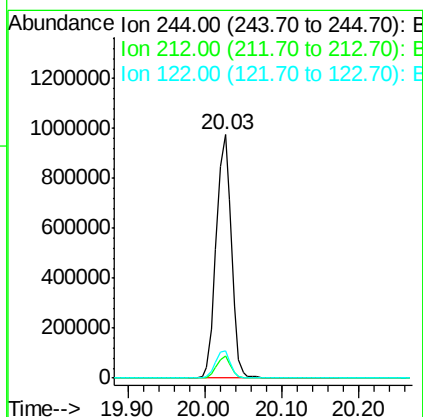

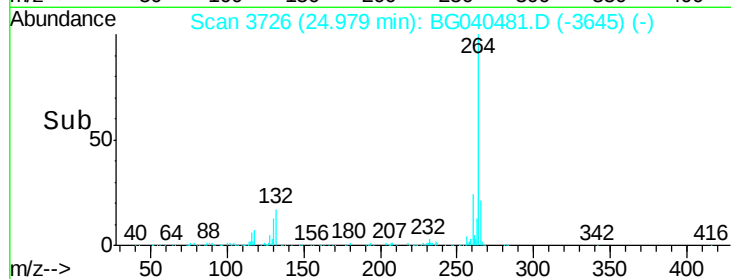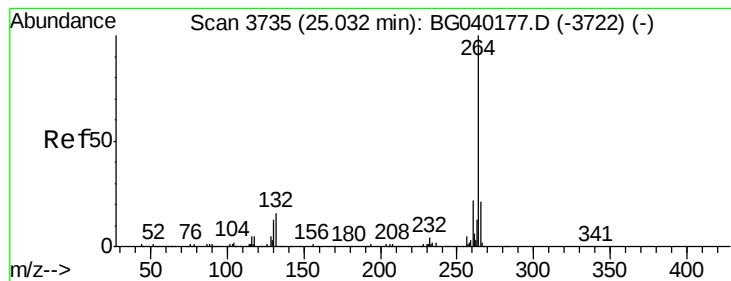

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.98 min Scan# 3726

Delta R.T. -0.05 min

Lab File: BG040481.D

Acq: 15 Apr 2019 15:38

Instrument :

BNA_G

ClientSampleId :

TP-11-D

Tgt Ion: 264 Resp: 346918

Ion Ratio Lower Upper

264 100

260 23.7 17.9 26.9

265 20.6 16.8 25.2

