


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041519\
 Data File : BG040494.D
 Acq On : 16 Apr 2019 00:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Apr 13 00:33:11 2019

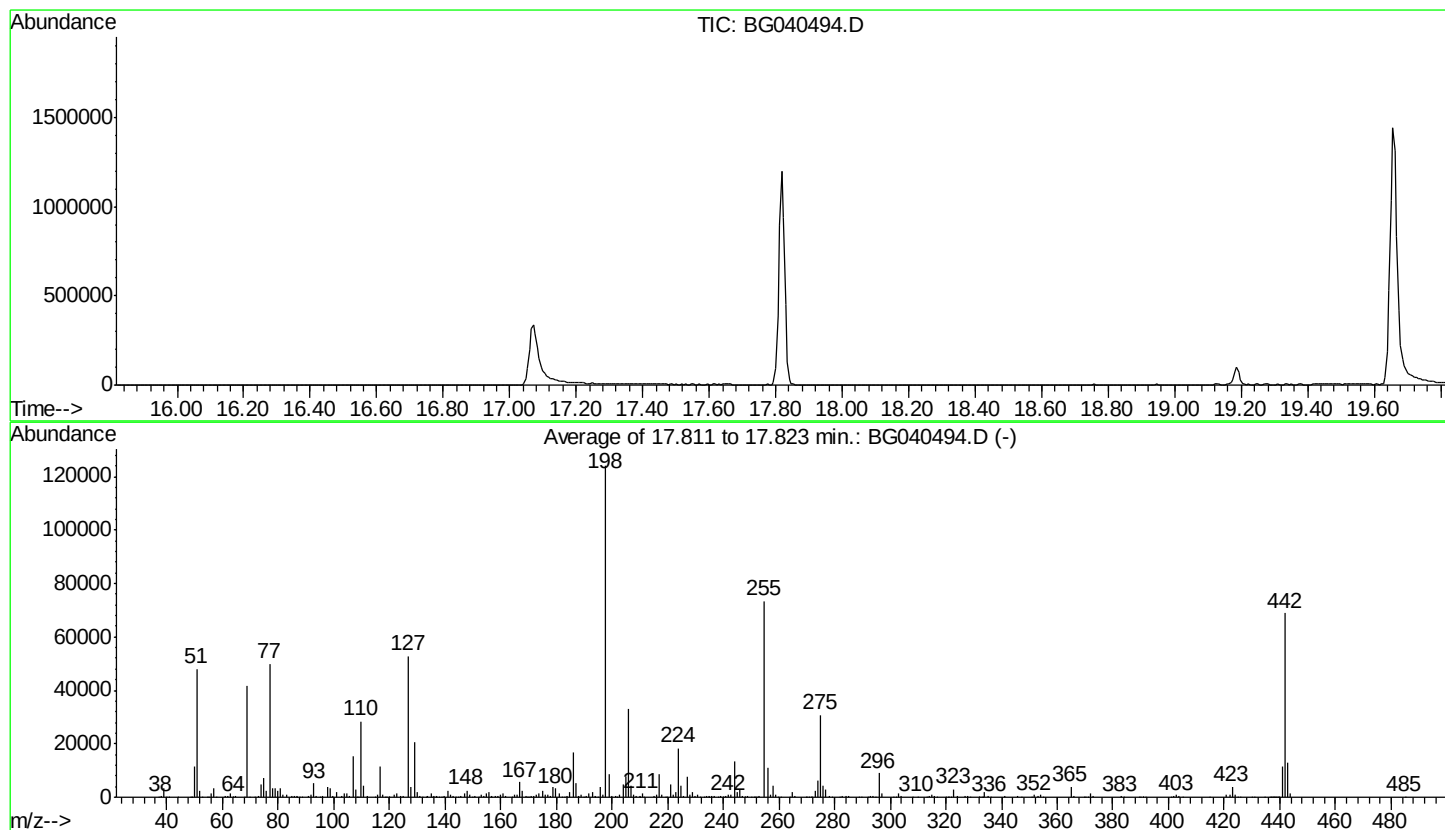

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	47989	PASS
68	69	0.00	2	0.5	211	PASS
69	198	0.00	100	33.7	41856	PASS
70	69	0.00	2	0.5	211	PASS
127	198	10	80	42.6	52898	PASS
197	198	0.00	2	0.7	856	PASS
198	198	100	100	100.0	124098	PASS
199	198	5	9	6.8	8500	PASS
275	198	10	60	24.8	30837	PASS
365	198	1	100	3.3	4040	PASS
441	198	0.01	100	9.3	11535	PASS
442	198	50	100	55.5	68896	PASS
443	442	15	24	18.9	13011	PASS