


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG041520\
 Data File : BG044978.D
 Acq On : 15 Apr 2020 12:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 15 17:57:00 2020

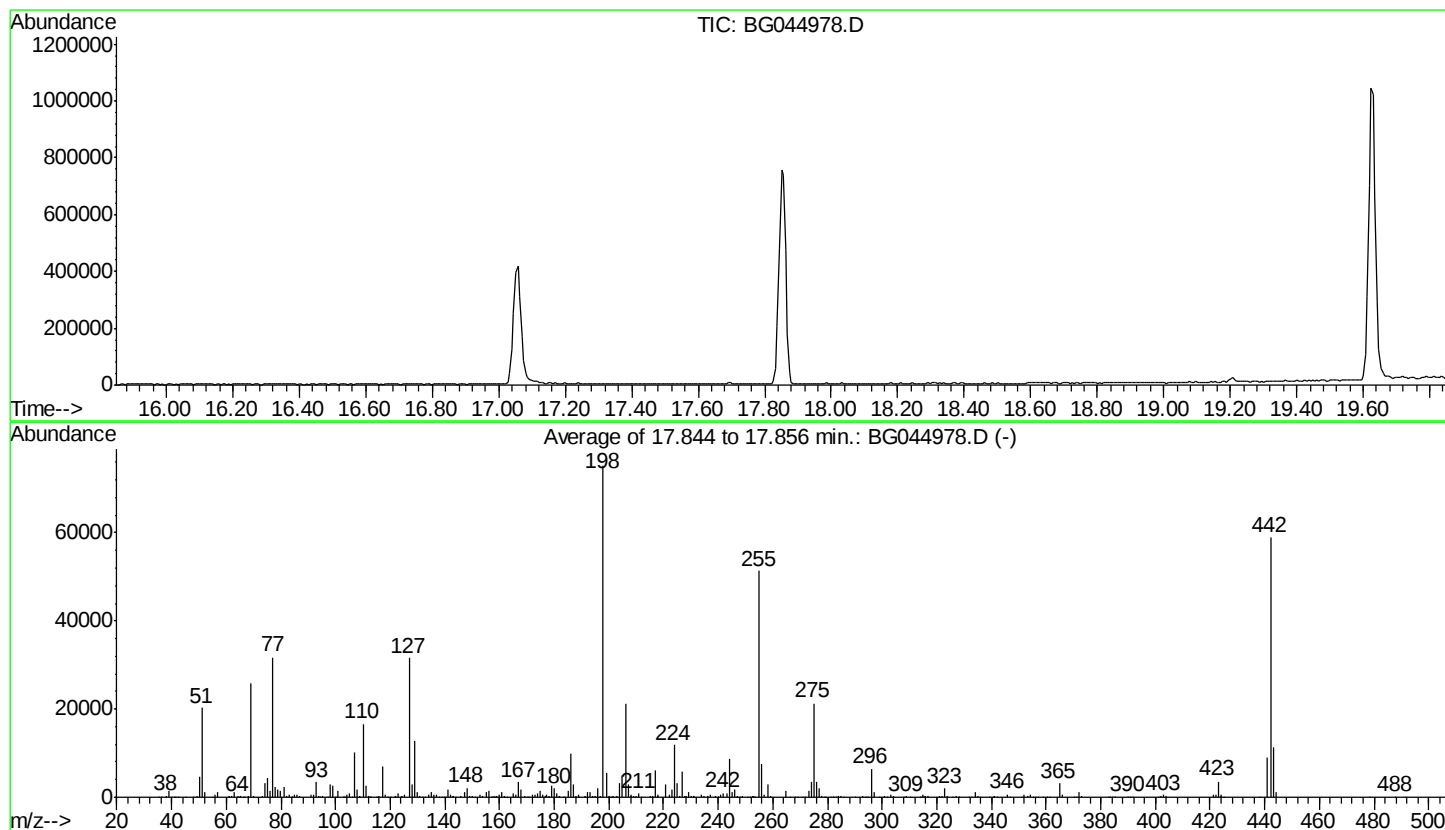

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	20266	PASS
68	69	0.00	2	1.6	407	PASS
69	198	0.00	100	34.5	25936	PASS
70	69	0.00	2	0.7	175	PASS
127	198	10	80	42.1	31648	PASS
197	198	0.00	2	0.4	307	PASS
198	198	100	100	100.0	75240	PASS
199	198	5	9	7.2	5410	PASS
275	198	10	60	28.2	21213	PASS
365	198	1	100	4.2	3152	PASS
441	198	0.01	100	12.0	9033	PASS
442	198	50	100	78.3	58946	PASS
443	442	15	24	19.0	11229	PASS