


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG041520\
 Data File : BG044987.D
 Acq On : 15 Apr 2020 18:17
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 15 17:57:00 2020

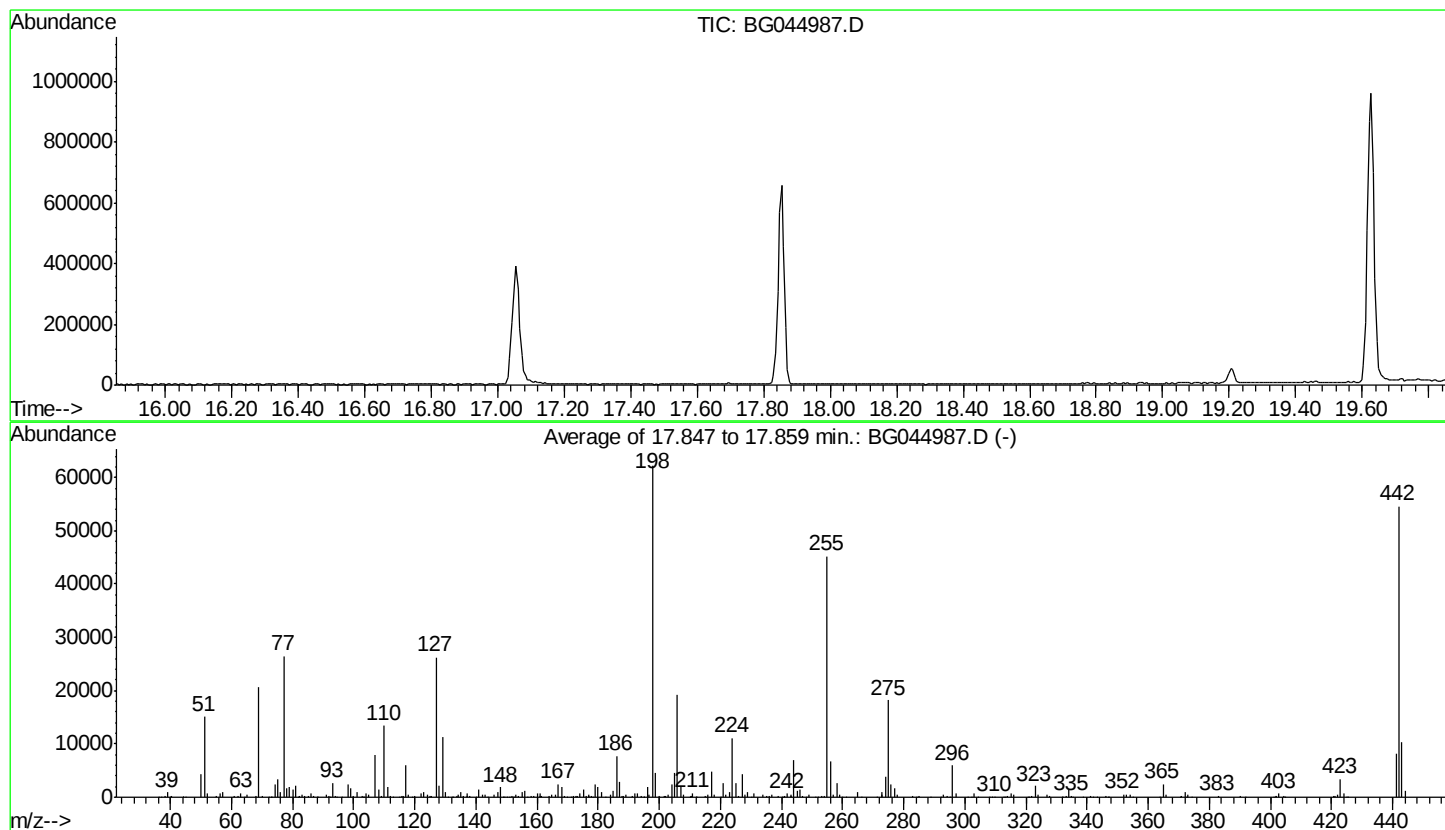

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	15053	PASS
68	69	0.00	2	1.2	251	PASS
69	198	0.00	100	33.2	20628	PASS
70	69	0.00	2	0.7	153	PASS
127	198	10	80	42.2	26266	PASS
197	198	0.00	2	0.6	394	PASS
198	198	100	100	100.0	62218	PASS
199	198	5	9	7.3	4571	PASS
275	198	10	60	29.3	18220	PASS
365	198	1	100	4.0	2507	PASS
441	198	0.01	100	13.1	8142	PASS
442	198	50	100	87.7	54544	PASS
443	442	15	24	19.1	10434	PASS